



ORE RESEARCH & EXPLORATION P/L ABN 28 006 859 856
37A Hosie Street · Bayswater North · VIC 3153 · AUSTRALIA
☎ 61 3 9729 0333 ☎ 61 3 9729 8338
📧 info@oreas.com 🌐 www.oreas.com

CERTIFICATE OF ANALYSIS FOR
CERTIFIED REFERENCE MATERIAL
OREAS 317
Zinc-Lead-Silver Ore
(Northern Queensland, Australia)

Statistics for *Key Economic Elements.


Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5% window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
4-Acid Digestion											
Ag, ppm	232	8	216	247	208	255	3.38%	6.77%	10.15%	220	243
Pb, wt.%	12.13	0.466	11.20	13.06	10.73	13.53	3.84%	7.68%	11.53%	11.52	12.74
Zn, wt.%	17.45	0.383	16.68	18.21	16.30	18.60	2.20%	4.39%	6.59%	16.57	18.32

*See Table 1 for full list of certified values;

SI unit equivalents: ppm (parts per million; 1×10^6) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.



Document: COA-1566-OREAS 317-R0

(Template: BUP-70-10-01 Rev:2.0)

30-March-2022

TABLE OF CONTENTS

INTRODUCTION	8
SOURCE MATERIAL.....	8
PERFORMANCE GATES	8
COMMUNITION AND HOMOGENISATION PROCEDURES	9
PHYSICAL PROPERTIES	9
ANALYTICAL PROGRAM.....	9
STATISTICAL ANALYSIS.....	10
Certified Values and their uncertainty intervals.....	10
Indicative (uncertified) values.....	10
Standard Deviation.....	10
Homogeneity Evaluation	16
PARTICIPATING LABORATORIES.....	17
PREPARER	17
METROLOGICAL TRACEABILITY	21
COMMUTABILITY	21
INTENDED USE	21
PERIOD OF VALIDITY & STORAGE INSTRUCTIONS.....	22
INSTRUCTIONS FOR HANDLING & CORRECT USE.....	22
DOCUMENT HISTORY	23
QMS CERTIFICATION	24
CERTIFYING OFFICER.....	24
LEGAL NOTICE.....	24
REFERENCES	24

LIST OF TABLES

Table 1. Certified Values and Performance Gates for OREAS 317.....	3
Table 2. Physical properties of OREAS 317.....	9
Table 3. Indicative Values for OREAS 317.....	11
Table 4. 95% Uncertainty & Tolerance Limits for OREAS 317.....	12

LIST OF FIGURES

Figure 1. Ag by 4-acid digestion in OREAS 317	18
Figure 2. Pb by 4-acid digestion in OREAS 317	19
Figure 3. Zn by 4-acid digestion in OREAS 317	20

Table 1. Certified Values and Performance Gates for OREAS 317.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5% window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
Oxidising Fusion XRF											
Al ₂ O ₃ , wt. %	5.79	0.112	5.56	6.01	5.45	6.12	1.93%	3.87%	5.80%	5.50	6.08
As, ppm	249	70	109	390	38	460	28.21%	56.42%	84.63%	237	262
BaO, wt. %	0.365	0.026	0.313	0.416	0.288	0.442	7.05%	14.10%	21.15%	0.347	0.383
CaO, wt. %	0.828	0.051	0.726	0.929	0.675	0.980	6.15%	12.29%	18.44%	0.786	0.869
Cu, wt. %	0.421	0.035	0.351	0.491	0.316	0.527	8.36%	16.71%	25.07%	0.400	0.442
Fe, wt. %	6.92	0.150	6.62	7.21	6.47	7.36	2.16%	4.33%	6.49%	6.57	7.26
K ₂ O, wt. %	1.95	0.125	1.70	2.20	1.58	2.32	6.39%	12.77%	19.16%	1.85	2.05
MgO, wt. %	0.704	0.086	0.533	0.875	0.447	0.961	12.15%	24.30%	36.44%	0.669	0.739
Mn, wt. %	0.693	0.025	0.643	0.744	0.618	0.769	3.63%	7.26%	10.89%	0.659	0.728
P ₂ O ₅ , wt. %	0.072	0.011	0.050	0.093	0.040	0.104	14.86%	29.72%	44.58%	0.068	0.075
Pb, wt. %	12.42	0.445	11.53	13.31	11.09	13.76	3.58%	7.17%	10.75%	11.80	13.04
S, wt. %	14.96	0.333	14.29	15.62	13.96	15.96	2.23%	4.45%	6.68%	14.21	15.71
SiO ₂ , wt. %	31.15	0.677	29.80	32.51	29.12	33.18	2.17%	4.34%	6.52%	29.60	32.71
TiO ₂ , wt. %	0.244	0.014	0.215	0.273	0.201	0.288	5.91%	11.81%	17.72%	0.232	0.257
Zn, wt. %	17.28	0.213	16.85	17.71	16.64	17.92	1.23%	2.46%	3.69%	16.42	18.14
Thermogravimetry											
LOI ¹⁰⁰⁰ , wt. %	11.54	0.324	10.89	12.19	10.57	12.51	2.80%	5.61%	8.41%	10.96	12.12
Infrared Combustion											
C, wt. %	1.91	0.046	1.82	2.00	1.77	2.05	2.38%	4.77%	7.15%	1.81	2.01
S, wt. %	15.17	0.495	14.18	16.16	13.69	16.66	3.26%	6.53%	9.79%	14.41	15.93
Borate / Peroxide Fusion ICP											
Ag, ppm	231	8	216	247	208	254	3.35%	6.71%	10.06%	220	243
Al, wt. %	3.07	0.143	2.79	3.36	2.64	3.50	4.65%	9.30%	13.95%	2.92	3.22
As, ppm	243	13	216	270	203	283	5.48%	10.96%	16.44%	231	255
B, ppm	47.1	16.8	13.5	80.7	0.0	97.5	35.65%	71.31%	106.96 %	44.8	49.5
Ba, wt. %	0.317	0.014	0.290	0.345	0.276	0.359	4.32%	8.64%	12.96%	0.302	0.333
Be, ppm	1.78	0.34	1.09	2.47	0.75	2.81	19.34%	38.68%	58.02%	1.69	1.87
Bi, ppm	42.4	3.02	36.4	48.5	33.4	51.5	7.11%	14.21%	21.32%	40.3	44.6
Ca, wt. %	0.564	0.040	0.484	0.644	0.444	0.684	7.11%	14.23%	21.34%	0.536	0.592
Cd, ppm	379	16	347	411	331	427	4.24%	8.47%	12.71%	360	398
Ce, ppm	41.7	1.76	38.2	45.2	36.4	47.0	4.22%	8.44%	12.66%	39.6	43.8
Co, ppm	12.9	2.3	8.2	17.5	5.9	19.8	18.06%	36.12%	54.18%	12.2	13.5
Cr, ppm	72	15	42	102	27	117	20.79%	41.58%	62.37%	69	76
Cs, ppm	1.94	0.194	1.56	2.33	1.36	2.52	9.98%	19.95%	29.93%	1.85	2.04
Cu, wt. %	0.410	0.014	0.381	0.439	0.367	0.453	3.49%	6.98%	10.48%	0.390	0.431
Dy, ppm	2.39	0.155	2.08	2.70	1.92	2.86	6.49%	12.98%	19.48%	2.27	2.51
Er, ppm	1.41	0.085	1.24	1.58	1.15	1.66	6.07%	12.13%	18.20%	1.34	1.48
Eu, ppm	0.70	0.08	0.54	0.87	0.45	0.96	12.02%	24.04%	36.05%	0.67	0.74
Fe, wt. %	6.90	0.207	6.49	7.32	6.28	7.52	2.99%	5.99%	8.98%	6.56	7.25
Ga, ppm	11.8	1.3	9.2	14.4	7.9	15.7	11.00%	22.01%	33.01%	11.2	12.4

SI unit equivalents: ppm (parts per million; 1×10^6) \equiv mg/kg; wt. % (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Table 1. continued.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5% window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
Borate / Peroxide Fusion ICP continued											
Gd, ppm	2.88	0.185	2.51	3.25	2.32	3.43	6.44%	12.88%	19.32%	2.73	3.02
Ge, ppm	3.35	0.73	1.90	4.81	1.17	5.54	21.68%	43.36%	65.04%	3.19	3.52
Ho, ppm	0.48	0.06	0.37	0.59	0.31	0.65	11.81%	23.62%	35.43%	0.46	0.50
In, ppm	1.29	0.14	1.01	1.58	0.87	1.72	10.94%	21.87%	32.81%	1.23	1.36
K, wt. %	1.65	0.055	1.54	1.76	1.49	1.82	3.34%	6.69%	10.03%	1.57	1.73
La, ppm	19.5	2.2	15.2	23.8	13.0	25.9	11.07%	22.15%	33.22%	18.5	20.4
Li, ppm	14.8	1.7	11.5	18.1	9.8	19.8	11.20%	22.40%	33.60%	14.1	15.5
Mg, wt. %	0.401	0.016	0.370	0.433	0.354	0.448	3.92%	7.84%	11.77%	0.381	0.421
Mn, wt. %	0.695	0.026	0.643	0.746	0.617	0.772	3.72%	7.44%	11.17%	0.660	0.729
Mo, ppm	44.0	3.77	36.4	51.5	32.6	55.3	8.58%	17.16%	25.74%	41.8	46.2
Nb, ppm	5.71	0.72	4.28	7.14	3.56	7.85	12.53%	25.07%	37.60%	5.42	5.99
Nd, ppm	17.9	0.80	16.3	19.5	15.5	20.3	4.46%	8.93%	13.39%	17.0	18.8
Ni, ppm	104	15	74	135	58	151	14.75%	29.51%	44.26%	99	110
P, wt. %	0.030	0.005	0.020	0.040	0.015	0.044	16.23%	32.46%	48.69%	0.028	0.031
Pb, wt. %	12.09	0.259	11.57	12.61	11.31	12.87	2.14%	4.29%	6.43%	11.48	12.69
Pr, ppm	4.54	0.234	4.07	5.00	3.84	5.24	5.15%	10.30%	15.45%	4.31	4.76
Rb, ppm	76	4.4	68	85	63	90	5.69%	11.38%	17.07%	73	80
S, wt. %	15.02	0.340	14.34	15.70	14.00	16.04	2.26%	4.53%	6.79%	14.27	15.77
Sb, ppm	253	11	231	275	220	285	4.33%	8.67%	13.00%	240	265
Se, ppm	< 20	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Si, wt. %	15.23	0.616	14.00	16.46	13.38	17.08	4.05%	8.09%	12.14%	14.47	15.99
Sm, ppm	3.39	0.36	2.67	4.12	2.30	4.49	10.73%	21.46%	32.20%	3.23	3.56
Sr, ppm	121	9	104	138	95	146	7.10%	14.20%	21.30%	115	127
Tb, ppm	0.40	0.014	0.37	0.43	0.36	0.44	3.48%	6.95%	10.43%	0.38	0.42
Th, ppm	7.14	0.308	6.53	7.76	6.22	8.07	4.32%	8.63%	12.95%	6.79	7.50
Ti, wt. %	0.143	0.009	0.126	0.160	0.118	0.169	5.95%	11.90%	17.85%	0.136	0.151
Tl, ppm	17.2	0.72	15.8	18.6	15.0	19.4	4.20%	8.40%	12.60%	16.3	18.1
Tm, ppm	0.20	0.03	0.14	0.27	0.11	0.30	15.88%	31.75%	47.63%	0.19	0.21
U, ppm	4.59	0.374	3.84	5.34	3.47	5.71	8.14%	16.29%	24.43%	4.36	4.82
V, ppm	70	5.7	59	81	53	87	8.12%	16.23%	24.35%	67	74
Y, ppm	12.7	1.5	9.7	15.7	8.2	17.1	11.71%	23.41%	35.12%	12.0	13.3
Yb, ppm	1.40	0.14	1.12	1.69	0.97	1.83	10.21%	20.43%	30.64%	1.33	1.47
Zn, wt. %	17.38	0.531	16.32	18.44	15.79	18.97	3.05%	6.11%	9.16%	16.51	18.25
Zr, ppm	60	10	39	80	29	91	17.07%	34.14%	51.20%	57	63
4-Acid Digestion											
Ag, ppm	232	8	216	247	208	255	3.38%	6.77%	10.15%	220	243
Al, wt. %	3.02	0.177	2.67	3.38	2.49	3.56	5.87%	11.74%	17.60%	2.87	3.18
As, ppm	237	21	195	278	174	299	8.82%	17.63%	26.45%	225	248
Be, ppm	1.48	0.105	1.27	1.69	1.16	1.79	7.09%	14.18%	21.27%	1.40	1.55
Bi, ppm	44.4	2.31	39.8	49.0	37.5	51.3	5.20%	10.40%	15.59%	42.2	46.6

SI unit equivalents: ppm (parts per million; 1×10^6) \equiv mg/kg; wt. % (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Table 1. continued.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5% window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
4-Acid Digestion continued											
Ca, wt. %	0.583	0.035	0.513	0.653	0.478	0.688	6.01%	12.01%	18.02%	0.554	0.612
Cd, ppm	374	28	318	429	291	457	7.41%	14.82%	22.22%	355	393
Ce, ppm	37.2	1.89	33.4	41.0	31.5	42.9	5.09%	10.19%	15.28%	35.3	39.0
Co, ppm	12.5	1.5	9.4	15.6	7.9	17.1	12.25%	24.50%	36.75%	11.9	13.1
Cr, ppm	64	6.3	52	77	46	83	9.70%	19.41%	29.11%	61	68
Cs, ppm	1.86	0.23	1.40	2.33	1.17	2.56	12.46%	24.92%	37.39%	1.77	1.96
Cu, wt. %	0.413	0.017	0.379	0.446	0.362	0.463	4.10%	8.21%	12.31%	0.392	0.433
Dy, ppm	2.18	0.25	1.68	2.68	1.44	2.93	11.41%	22.82%	34.22%	2.07	2.29
Er, ppm	1.13	0.20	0.73	1.53	0.54	1.73	17.58%	35.15%	52.73%	1.08	1.19
Eu, ppm	0.61	0.08	0.46	0.76	0.38	0.83	12.33%	24.67%	37.00%	0.58	0.64
Fe, wt. %	6.83	0.361	6.11	7.55	5.75	7.91	5.28%	10.57%	15.85%	6.49	7.17
Ga, ppm	10.7	1.3	8.1	13.4	6.7	14.7	12.40%	24.80%	37.20%	10.2	11.2
Gd, ppm	2.63	0.28	2.06	3.20	1.77	3.48	10.83%	21.67%	32.50%	2.50	2.76
Hf, ppm	1.33	0.14	1.05	1.60	0.91	1.74	10.39%	20.79%	31.18%	1.26	1.39
Ho, ppm	0.40	0.05	0.30	0.51	0.25	0.56	12.94%	25.89%	38.83%	0.38	0.42
In, ppm	1.18	0.13	0.91	1.45	0.78	1.59	11.41%	22.82%	34.22%	1.12	1.24
K, wt. %	1.62	0.048	1.52	1.71	1.47	1.76	2.98%	5.96%	8.93%	1.54	1.70
La, ppm	15.9	1.9	12.1	19.7	10.1	21.6	12.05%	24.11%	36.16%	15.1	16.7
Li, ppm	14.1	1.39	11.3	16.9	9.9	18.2	9.86%	19.72%	29.59%	13.4	14.8
Lu, ppm	0.17	0.02	0.13	0.21	0.11	0.23	11.24%	22.49%	33.73%	0.16	0.18
Mg, wt. %	0.388	0.024	0.339	0.437	0.314	0.461	6.30%	12.61%	18.91%	0.368	0.407
Mn, wt. %	0.679	0.031	0.616	0.742	0.585	0.774	4.63%	9.27%	13.90%	0.645	0.713
Mo, ppm	41.5	1.64	38.2	44.8	36.6	46.4	3.96%	7.92%	11.89%	39.4	43.6
Na, wt. %	0.061	0.009	0.043	0.079	0.034	0.088	14.82%	29.63%	44.45%	0.058	0.064
Nd, ppm	15.8	1.53	12.8	18.9	11.3	20.4	9.63%	19.26%	28.89%	15.0	16.6
Ni, ppm	101	8	85	117	77	124	7.79%	15.57%	23.36%	96	106
P, wt. %	0.030	0.003	0.025	0.036	0.022	0.039	9.07%	18.14%	27.21%	0.029	0.032
Pb, wt. %	12.13	0.466	11.20	13.06	10.73	13.53	3.84%	7.68%	11.53%	11.52	12.74
Pr, ppm	4.29	0.174	3.94	4.64	3.77	4.81	4.05%	8.10%	12.15%	4.08	4.51
Rb, ppm	73	6.3	60	86	54	92	8.65%	17.30%	25.96%	69	77
Re, ppm	0.096	0.019	0.058	0.133	0.039	0.152	19.69%	39.39%	59.08%	0.091	0.100
S, wt. %	14.78	0.610	13.56	15.99	12.95	16.60	4.13%	8.25%	12.38%	14.04	15.51
Sb, ppm	224	35	155	293	121	328	15.39%	30.78%	46.18%	213	235
Sc, ppm	5.31	0.63	4.06	6.56	3.44	7.19	11.77%	23.55%	35.32%	5.05	5.58
Se, ppm	4.98	1.06	2.86	7.10	1.80	8.17	21.31%	42.62%	63.93%	4.73	5.23
Sm, ppm	3.22	0.262	2.69	3.74	2.43	4.00	8.16%	16.32%	24.48%	3.05	3.38
Sn, ppm	3.61	0.62	2.37	4.84	1.76	5.45	17.09%	34.17%	51.26%	3.43	3.79
Sr, ppm	101	9	84	119	75	128	8.60%	17.21%	25.81%	96	107
Tb, ppm	0.37	0.033	0.31	0.44	0.27	0.47	8.79%	17.58%	26.38%	0.35	0.39
Te, ppm	0.82	0.17	0.49	1.15	0.32	1.32	20.17%	40.34%	60.51%	0.78	0.86

SI unit equivalents: ppm (parts per million; 1×10^6) \equiv mg/kg; wt. % (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Table 1. continued.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5% window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
4-Acid Digestion continued											
Th, ppm	6.17	0.87	4.42	7.92	3.55	8.79	14.16%	28.31%	42.47%	5.86	6.48
Ti, wt. %	0.106	0.024	0.059	0.154	0.035	0.178	22.45%	44.89%	67.34%	0.101	0.111
Tl, ppm	17.8	1.48	14.8	20.8	13.4	22.3	8.33%	16.66%	24.99%	16.9	18.7
Tm, ppm	0.18	0.02	0.14	0.22	0.12	0.24	11.25%	22.50%	33.75%	0.17	0.19
U, ppm	4.49	0.253	3.99	5.00	3.73	5.25	5.63%	11.27%	16.90%	4.27	4.72
V, ppm	67	3.2	61	73	58	77	4.73%	9.46%	14.19%	64	70
W, ppm	1.71	0.25	1.22	2.21	0.97	2.46	14.50%	29.00%	43.50%	1.63	1.80
Y, ppm	10.3	1.4	7.4	13.1	5.9	14.6	14.09%	28.19%	42.28%	9.7	10.8
Yb, ppm	1.18	0.23	0.73	1.63	0.50	1.86	19.20%	38.40%	57.60%	1.12	1.24
Zn, wt. %	17.45	0.383	16.68	18.21	16.30	18.60	2.20%	4.39%	6.59%	16.57	18.32
Zr, ppm	40.9	3.91	33.1	48.7	29.2	52.6	9.55%	19.10%	28.65%	38.8	42.9
Aqua Regia Digestion											
Ag, ppm	232	7	217	247	210	254	3.20%	6.40%	9.59%	220	243
Al, wt. %	0.508	0.095	0.317	0.698	0.222	0.794	18.78%	37.55%	56.33%	0.482	0.533
As, ppm	242	16	211	274	195	290	6.51%	13.03%	19.54%	230	255
Be, ppm	0.48	0.06	0.36	0.60	0.30	0.66	12.63%	25.25%	37.88%	0.46	0.50
Bi, ppm	44.1	2.70	38.7	49.5	36.0	52.2	6.11%	12.23%	18.34%	41.9	46.3
Ca, wt. %	0.575	0.032	0.512	0.638	0.480	0.670	5.50%	10.99%	16.49%	0.546	0.604
Cd, ppm	369	27	314	424	287	452	7.44%	14.87%	22.31%	351	388
Ce, ppm	27.0	5.1	16.8	37.2	11.7	42.3	18.91%	37.83%	56.74%	25.6	28.3
Co, ppm	10.3	2.5	5.3	15.2	2.8	17.7	24.12%	48.25%	72.37%	9.8	10.8
Cr, ppm	24.1	1.81	20.5	27.7	18.7	29.5	7.50%	15.01%	22.51%	22.9	25.3
Cs, ppm	0.70	0.08	0.53	0.87	0.45	0.96	12.02%	24.03%	36.05%	0.67	0.74
Cu, wt. %	0.422	0.020	0.382	0.463	0.361	0.483	4.80%	9.60%	14.40%	0.401	0.443
Dy, ppm	1.10	0.19	0.71	1.48	0.52	1.67	17.61%	35.23%	52.84%	1.04	1.15
Er, ppm	0.50	0.12	0.26	0.74	0.14	0.86	24.03%	48.05%	72.08%	0.47	0.52
Eu, ppm	0.38	0.024	0.33	0.43	0.31	0.45	6.27%	12.53%	18.80%	0.36	0.40
Fe, wt. %	6.78	0.341	6.10	7.46	5.75	7.80	5.03%	10.06%	15.08%	6.44	7.12
Ga, ppm	4.14	0.64	2.86	5.43	2.22	6.07	15.48%	30.96%	46.44%	3.94	4.35
Gd, ppm	1.57	0.33	0.91	2.23	0.58	2.56	20.97%	41.94%	62.92%	1.49	1.65
Hf, ppm	0.32	0.06	0.19	0.45	0.13	0.51	20.10%	40.20%	60.31%	0.30	0.34
Hg, ppm	6.01	0.67	4.67	7.35	4.00	8.02	11.17%	22.35%	33.52%	5.71	6.31
Ho, ppm	0.20	0.020	0.16	0.24	0.14	0.26	9.72%	19.44%	29.16%	0.19	0.21
In, ppm	1.15	0.113	0.93	1.38	0.82	1.49	9.75%	19.49%	29.24%	1.10	1.21
K, wt. %	0.188	0.033	0.121	0.255	0.088	0.289	17.76%	35.52%	53.28%	0.179	0.198
La, ppm	10.8	2.4	6.1	15.6	3.7	17.9	21.82%	43.65%	65.47%	10.3	11.4
Li, ppm	5.36	1.08	3.20	7.52	2.12	8.60	20.14%	40.28%	60.42%	5.09	5.63
Lu, ppm	0.071	0.011	0.049	0.094	0.037	0.106	15.90%	31.80%	47.70%	0.068	0.075
Mg, wt. %	0.264	0.018	0.227	0.301	0.209	0.319	6.99%	13.98%	20.96%	0.251	0.277
Mn, wt. %	0.664	0.046	0.572	0.755	0.527	0.800	6.88%	13.75%	20.63%	0.630	0.697

SI unit equivalents: ppm (parts per million; 1×10^6) \equiv mg/kg; wt. % (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Table 1. continued.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5% window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
Aqua Regia Digestion continued											
Mo, ppm	41.1	2.82	35.4	46.7	32.6	49.5	6.87%	13.73%	20.60%	39.0	43.1
Nd, ppm	10.5	0.66	9.2	11.8	8.5	12.5	6.27%	12.53%	18.80%	10.0	11.0
Ni, ppm	99	7.0	85	113	78	120	7.04%	14.08%	21.13%	94	104
P, wt. %	0.029	0.002	0.025	0.033	0.022	0.036	7.68%	15.36%	23.04%	0.028	0.030
Pb, wt. %	12.19	0.298	11.59	12.78	11.29	13.08	2.44%	4.89%	7.33%	11.58	12.80
Pr, ppm	2.61	0.53	1.56	3.66	1.03	4.19	20.17%	40.33%	60.50%	2.48	2.74
Rb, ppm	11.4	2.9	5.5	17.3	2.5	20.2	25.94%	51.89%	77.83%	10.8	11.9
Re, ppm	0.11	0.01	0.08	0.13	0.07	0.14	10.09%	20.19%	30.28%	0.10	0.11
S, wt. %	14.92	0.675	13.57	16.27	12.89	16.94	4.52%	9.05%	13.57%	14.17	15.66
Sb, ppm	200	19	163	238	144	257	9.37%	18.73%	28.10%	190	210
Sc, ppm	1.27	0.24	0.79	1.75	0.55	1.99	18.98%	37.95%	56.93%	1.21	1.33
Se, ppm	6.87	1.01	4.85	8.89	3.85	9.89	14.67%	29.35%	44.02%	6.53	7.21
Sm, ppm	1.86	0.36	1.14	2.58	0.78	2.94	19.37%	38.75%	58.12%	1.77	1.95
Sn, ppm	2.52	0.41	1.70	3.35	1.29	3.76	16.29%	32.58%	48.88%	2.40	2.65
Sr, ppm	21.2	3.2	14.9	27.5	11.7	30.6	14.90%	29.79%	44.69%	20.1	22.2
Ta, ppm	< 0.05	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Tb, ppm	0.23	0.03	0.17	0.29	0.14	0.32	13.27%	26.55%	39.82%	0.22	0.24
Te, ppm	0.86	0.16	0.54	1.19	0.37	1.36	18.93%	37.86%	56.79%	0.82	0.91
Th, ppm	5.07	0.423	4.22	5.92	3.80	6.34	8.35%	16.69%	25.04%	4.82	5.32
Ti, wt. %	0.010	0.001	0.008	0.011	0.007	0.012	8.62%	17.25%	25.87%	0.009	0.010
Tl, ppm	10.9	0.89	9.1	12.6	8.2	13.5	8.17%	16.33%	24.50%	10.3	11.4
Tm, ppm	0.057	0.025	0.006	0.108	0.000	0.133	44.53%	89.06%	133.59 oz	0.054	0.060
U, ppm	3.55	0.293	2.96	4.13	2.67	4.42	8.25%	16.50%	24.75%	3.37	3.72
V, ppm	16.2	3.1	10.0	22.5	6.9	25.6	19.19%	38.37%	57.56%	15.4	17.0
W, ppm	0.75	0.13	0.48	1.01	0.35	1.15	17.84%	35.68%	53.52%	0.71	0.78
Y, ppm	4.65	0.92	2.82	6.49	1.90	7.40	19.69%	39.39%	59.08%	4.42	4.89
Yb, ppm	0.42	0.12	0.18	0.67	0.05	0.79	29.03%	58.06%	87.08%	0.40	0.44
Zn, wt. %	17.49	0.398	16.70	18.29	16.30	18.69	2.28%	4.55%	6.83%	16.62	18.37
Zr, ppm	11.5	3.1	5.3	17.7	2.2	20.8	27.04%	54.09%	81.13%	10.9	12.0

SI unit equivalents: ppm (parts per million; 1×10^6) \equiv mg/kg; wt. % (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

INTRODUCTION

OREAS reference materials are intended to provide a low-cost method of evaluating and improving the quality of analysis of geological samples. To the geologist they provide a means of implementing quality control in analytical data sets generated in exploration from the grass roots level through to prospect evaluation, and in grade control at mining operations. To the analyst they provide an effective means of calibrating analytical equipment, assessing new techniques and routinely monitoring in-house procedures. OREAS reference materials enable users to successfully achieve process control of these tasks because the observed variance from repeated analysis has its origin almost exclusively in the analytical process rather than the reference material itself. In evaluating laboratory performance with this CRM, the section headed 'Instructions for correct use' should be read carefully.

Table 1 provides performance gate intervals for the certified values, Table 2 provides some indicative physical properties, Table 3 shows indicative values and Table 4 presents the 95% expanded uncertainty and tolerance limits for all certified values. Tabulated results of all analytes together with uncorrected means, medians, standard deviations, relative standard deviations and per cent deviation of lab means from the corrected mean of means (PDM³) are presented in the detailed certification data for this CRM (**OREAS 317-DataPack.1.0.220329_165941.xlsx**).

Comparisons of interlaboratory bias and precision are graphically presented in scatter plots for Ag, Pb and Zn by 4-acid digestion (Figures 1 to 3, respectively) together with $\pm 3SD$ (magenta) and certified value (green line). Accepted individual results are coloured blue and individual and dataset outliers are identified in red and violet, respectively.

SOURCE MATERIAL

OREAS 317 has been prepared from a blend of barren black slate and various Zn-Pb-Ag ore and concentrate materials. This includes materials from the Dugald River, Black Star and Cannington deposits located in Northern Queensland, Australia.

PERFORMANCE GATES

Table 1 above shows intervals calculated for two and three standard deviations. As a guide these intervals may be regarded as warning or rejection for multiple 2SD outliers, or rejection for individual 3SD outliers in QC monitoring, although their precise application should be at the discretion of the QC manager concerned (also see 'Intended Use' section below). Westgard Rules extend the basics of single-rule QC monitoring using multi-rules (for more information visit www.westgard.com/mltirule.htm). A second method utilises a 5% window calculated directly from the certified value. For information on the calculation of standard deviations see the 'Statistical Analysis' section below.

Standard deviation is also shown in relative percent for one, two and three relative standard deviations (1RSD, 2RSD and 3RSD) to facilitate an appreciation of the magnitude of these numbers and a comparison with the 5% window. Caution should be exercised when concentration levels approach lower limits of detection of the analytical methods employed as performance gates calculated from standard deviations tend to be excessively wide whereas those determined by the 5% method are too narrow. One

approach used at commercial laboratories is to set the acceptance criteria at twice the detection level (DL) \pm 10%.

i.e., Certified Value \pm 10% \pm 2DL (adapted from Govett, 1983).

COMMINUTION AND HOMOGENISATION PROCEDURES

The material constituting OREAS 317 was prepared in the following manner:

- Drying of ores and concentrates to constant mass at 85°C;
- Drying of barren slate to constant mass at 105°C;
- Crushing and multi-stage milling of ores and concentrates to 100% minus 30 microns;
- Crushing and milling of barren slate to 98% minus 75 microns;
- Preliminary homogenisation and check assaying of ores and concentrates;
- Blending the barren slate, ores and concentrates in specific ratios to achieve target Zn, Pb and Ag values.
- Packaging into 10g units sealed under nitrogen in laminated foil pouches.

PHYSICAL PROPERTIES

OREAS 317 was tested at ORE Research & Exploration Pty Ltd's onsite facility for various physical properties. Table 2 presents these findings that should be used for informational purposes only.

Table 2. Physical properties of OREAS 317.

Bulk Density (g/L)	Moisture%	Munsell Notation [‡]	Munsell Color [‡]
776	0.81	5Y 3/2	Olive Gray

[‡]The Munsell Rock Color Chart helps geologists and archeologists communicate with colour more effectively by cross-referencing ISCC-NBS colour names with unique Munsell alpha-numeric colour notations for rock colour samples.

ANALYTICAL PROGRAM

Twenty-six commercial analytical laboratories participated in the program to certify the elements reported in Table 1. The following methods were employed:

- Majors & base metals by oxidising fusion with X-ray fluorescence finish (up to 20 laboratories depending on the element);
- Loss on ignition at 1000° Celsius (12 laboratories);
- Total Sulphur by infrared combustion furnace or C/S analyser;
- Full ICP-OES and MS elemental suites by peroxide fusion (up to 22 laboratories depending on the element);
- Full ICP-OES and MS elemental suites by 4-acid (HNO₃-HF-HClO₄-HCl) digestion (up to 22 laboratories depending on the element);
- Full ICP-OES and MS elemental suites by aqua regia digestion (up to 18 laboratories depending on the element).

For the round robin program ten 500g test units were taken at predetermined intervals during the bagging stage, immediately following homogenisation and are considered representative of the entire prepared batch. Six 20g pulp samples were submitted to each laboratory for analysis. The samples received by each laboratory were obtained by taking two samples from each of three separate 500g test units. This format enabled a nested ANOVA treatment of the results to evaluate homogeneity, i.e., to ascertain whether between-unit variance is greater than within-unit variance (see 'Homogeneity Evaluation' section below).

STATISTICAL ANALYSIS

Certified Values and their uncertainty intervals (Table 4) have been determined for each analyte following removal of individual, laboratory dataset (batch) and 3SD outliers (single iteration).

For individual outliers within a laboratory batch the z-score test is used in combination with a second method that determines the per cent deviation of the individual value from the batch median. Outliers in general are selected on the basis of z-scores > 2.5 and with per cent deviations (i) > 3 and (ii) more than three times the average absolute per cent deviation for the batch. In certain instances, statistician's prerogative has been employed in discriminating outliers.

Each laboratory data set mean is tested for outlying status based on z-score discrimination and rejected if > 2.5 . After individual and laboratory data set (batch) outliers have been eliminated a non-iterative 3 standard deviation filter is applied, with those values lying outside this window also relegated to outlying status.

Certified Values are the means of accepted laboratory means after outlier filtering and are the present best estimate of the true value.

The 95% Expanded Uncertainty provides a 95% probability that the true value of the analyte under consideration lies between the upper and lower limits and is calculated according to the method in ISO Guides [5,15]. All known or suspected sources of bias have been investigated or taken into account.

Indicative (uncertified) values (Table 3) are present where the number of laboratories reporting a particular analyte is insufficient (< 5) to support certification. These major and trace element characterisation values are presented for informational purposes only.

Standard Deviation intervals (Table 1) provide an indication of a level of performance that might reasonably be expected from a laboratory being monitored by this CRM in a QA/QC program. They take into account errors attributable to measurement uncertainty and CRM variability. For an effective CRM the contribution of the latter should be negligible in comparison to measurement errors. The Standard Deviation values include all sources of measurement uncertainty: between-lab variance, within-run variance (precision errors) and CRM variability.

In the application of SD's in monitoring performance it is important to note that not all laboratories function at the same level of proficiency and that different methods in use at a particular laboratory have differing levels of precision. Each laboratory has its own inherent SD (for a specific concentration level and analyte-method pair) based on the analytical

process and this SD is not directly related to the round robin program (see 'Instructions for Correct Use' section for more detail).

The SD for each analyte's certified value is calculated from the same filtered data set used to determine the certified value, i.e., after removal of all individual, lab dataset (batch) and 3SD outliers (single iteration). These outliers can only be removed after the absolute homogeneity of the CRM has been independently established, i.e., the outliers must be confidently deemed to be analytical rather than arising from inhomogeneity of the CRM. **The standard deviation is then calculated for each analyte from the pooled accepted analyses generated from the certification program.**

Table 3. Indicative Values for OREAS 317.

Constituent	Unit	Value	Constituent	Unit	Value	Constituent	Unit	Value
Borate Fusion XRF								
Ag	ppm	228	Hg	ppm	< 100	Se	ppm	< 100
Bi	ppm	88	In	ppm	< 100	Sn	ppm	< 100
Cd	ppm	413	La	ppm	< 90	SrO	ppm	153
Ce	ppm	88	Mo	ppm	< 50	Ta	ppm	< 100
Co	ppm	< 100	Na ₂ O	wt.%	0.674	Te	ppm	< 100
Cr ₂ O ₃	ppm	156	Nb	ppm	135	Tl	ppm	< 100
Cs	ppm	< 100	Ni	ppm	143	V ₂ O ₅	ppm	95
Ga	ppm	< 100	Rb	ppm	134	W	ppm	< 10
Ge	ppm	< 100	Sb	ppm	205	Y	ppm	< 39
Hf	ppm	< 80	Sc	ppm	< 100	Zr	ppm	200
Borate / Peroxide Fusion ICP								
Hf	ppm	1.68	Re	ppm	0.050	Ta	ppm	0.46
Lu	ppm	0.19	Sc	ppm	3.92	Te	ppm	1.51
Na	wt.%	0.058	Sn	ppm	4.81	W	ppm	1.56
4-Acid Digestion								
Ba	wt.%	0.082	Nb	ppm	2.95			
Ge	ppm	0.23	Ta	ppm	0.24			
Aqua Regia Digestion								
Au	ppm	0.332	Ge	ppm	0.15	Pd	ppb	59.6
B	ppm	14.3	Na	wt.%	0.013	Pt	ppb	< 5
Ba	wt.%	0.001	Nb	ppm	0.19			

SI unit equivalents: ppm (parts per million; $1 \times 10^6 \equiv \text{mg/kg}$; wt.% (weight per cent) \equiv % (mass fraction).

Note: the number of significant figures reported is not a reflection of the level of certainty of stated values. They are instead an artefact of ORE's in-house CRM-specific LIMS.

Table 4. 95% Uncertainty & Tolerance Limits for OREAS 317.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
Borate Fusion XRF					
Al ₂ O ₃ , Aluminium(III) oxide (wt.%)	5.79	5.70	5.87	5.73	5.85
As, Arsenic (ppm)	249	127	371	IND	IND
BaO, Barium oxide (wt.%)	0.365	0.344	0.386	0.351	0.379
CaO, Calcium oxide (wt.%)	0.828	0.793	0.863	0.813	0.842
Cu, Copper (wt.%)	0.421	0.398	0.444	0.410	0.432
Fe, Iron (wt.%)	6.92	6.81	7.02	6.86	6.98
K ₂ O, Potassium oxide (wt.%)	1.95	1.88	2.02	1.93	1.97
MgO, Magnesium oxide (wt.%)	0.704	0.652	0.756	0.686	0.722
Mn, Manganese (wt.%)	0.693	0.677	0.710	0.683	0.704
P ₂ O ₅ , Phosphorus(V) oxide (wt.%)	0.072	0.062	0.081	IND	IND
Pb, Lead (wt.%)	12.42	12.11	12.74	12.32	12.52
S, Sulphur (wt.%)	14.96	14.64	15.27	14.75	15.16
SiO ₂ , Silicon dioxide (wt.%)	31.15	30.69	31.62	30.90	31.40
TiO ₂ , Titanium dioxide (wt.%)	0.244	0.232	0.257	0.234	0.254
Zn, Zinc (wt.%)	17.28	17.10	17.46	17.18	17.38
Thermogravimetry					
LOI ¹⁰⁰⁰ , Loss On Ignition @1000°C (wt.%)	11.54	11.29	11.79	11.41	11.66
Infrared Combustion					
C, Carbon (wt.%)	1.91	1.88	1.94	1.89	1.93
S, Sulphur (wt.%)	15.17	14.80	15.54	15.01	15.33
Borate / Peroxide Fusion ICP					
Ag, Silver (ppm)	231	218	245	222	240
Al, Aluminium (wt.%)	3.07	2.98	3.17	2.98	3.16
As, Arsenic (ppm)	243	230	256	225	262
B, Boron (ppm)	47.1	19.1	75.1	IND	IND
Ba, Barium (wt.%)	0.317	0.304	0.331	0.310	0.324
Be, Beryllium (ppm)	1.78	1.19	2.37	IND	IND
Bi, Bismuth (ppm)	42.4	39.6	45.2	41.0	43.9
Ca, Calcium (wt.%)	0.564	0.526	0.602	0.526	0.602
Cd, Cadmium (ppm)	379	358	400	366	393
Ce, Cerium (ppm)	41.7	39.8	43.7	39.9	43.5
Co, Cobalt (ppm)	12.9	11.3	14.4	11.6	14.1
Cr, Chromium (ppm)	72	60	84	62	83
Cs, Caesium (ppm)	1.94	1.73	2.16	1.76	2.12
Cu, Copper (wt.%)	0.410	0.397	0.424	0.401	0.419
Dy, Dysprosium (ppm)	2.39	2.13	2.65	2.18	2.60
Er, Erbium (ppm)	1.41	1.29	1.53	1.37	1.45
Eu, Europium (ppm)	0.70	0.59	0.82	0.66	0.75
Fe, Iron (wt.%)	6.90	6.65	7.15	6.74	7.06
Ga, Gallium (ppm)	11.8	9.9	13.6	10.4	13.1
Gd, Gadolinium (ppm)	2.88	2.60	3.15	2.69	3.06

SI unit equivalents: ppm (parts per million; $1 \times 10^6 \equiv \text{mg/kg}$; wt.% (weight per cent) $\equiv \%$ (mass fraction).

Note: intervals may appear asymmetric due to rounding.

IND = indeterminate (due to limited reading resolution of the methods employed).

Table 4. continued.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
Borate / Peroxide Fusion ICP continued					
Ho, Holmium (ppm)	0.48	0.37	0.59	0.46	0.50
In, Indium (ppm)	1.29	1.16	1.42	IND	IND
K, Potassium (wt.%)	1.65	1.60	1.70	1.60	1.70
La, Lanthanum (ppm)	19.5	17.9	21.1	18.8	20.1
Li, Lithium (ppm)	14.8	13.0	16.6	IND	IND
Mg, Magnesium (wt.%)	0.401	0.386	0.417	0.386	0.416
Mn, Manganese (wt.%)	0.695	0.669	0.720	0.678	0.712
Mo, Molybdenum (ppm)	44.0	41.2	46.7	41.8	46.2
Nb, Niobium (ppm)	5.71	4.96	6.45	IND	IND
Nd, Neodymium (ppm)	17.9	17.0	18.8	17.1	18.7
Ni, Nickel (ppm)	104	89	120	98	111
P, Phosphorus (wt.%)	0.030	0.022	0.038	IND	IND
Pb, Lead (wt.%)	12.09	11.76	12.42	11.89	12.29
Pr, Praseodymium (ppm)	4.54	4.23	4.85	4.34	4.74
Rb, Rubidium (ppm)	76	70	83	74	79
S, Sulphur (wt.%)	15.02	14.74	15.30	14.59	15.45
Sb, Antimony (ppm)	253	238	267	241	264
Se, Selenium (ppm)	< 20	IND	IND	IND	0.0
Si, Silicon (wt.%)	15.23	14.73	15.73	14.78	15.68
Sm, Samarium (ppm)	3.39	2.97	3.82	3.16	3.63
Sr, Strontium (ppm)	121	115	126	117	124
Tb, Terbium (ppm)	0.40	0.37	0.43	0.37	0.44
Th, Thorium (ppm)	7.14	6.79	7.50	6.93	7.36
Ti, Titanium (wt.%)	0.143	0.135	0.151	0.135	0.151
Tl, Thallium (ppm)	17.2	16.5	17.9	16.3	18.0
Tm, Thulium (ppm)	0.20	0.14	0.27	IND	IND
U, Uranium (ppm)	4.59	4.19	4.99	4.45	4.74
V, Vanadium (ppm)	70	64	77	66	74
Y, Yttrium (ppm)	12.7	11.6	13.8	12.2	13.2
Yb, Ytterbium (ppm)	1.40	1.24	1.57	IND	IND
Zn, Zinc (wt.%)	17.38	16.95	17.80	16.93	17.83
Zr, Zirconium (ppm)	60	43	77	IND	IND
4-Acid Digestion					
Ag, Silver (ppm)	232	227	236	225	238
Al, Aluminium (wt.%)	3.02	2.92	3.13	2.95	3.09
As, Arsenic (ppm)	237	225	248	229	244
Be, Beryllium (ppm)	1.48	1.39	1.56	1.41	1.55
Bi, Bismuth (ppm)	44.4	43.0	45.8	43.2	45.5
Ca, Calcium (wt.%)	0.583	0.564	0.602	0.571	0.595
Cd, Cadmium (ppm)	374	359	388	367	380
Ce, Cerium (ppm)	37.2	34.0	40.3	35.6	38.8

SI unit equivalents: ppm (parts per million; 1×10^6) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

Note: intervals may appear asymmetric due to rounding.

IND = indeterminate (due to limited reading resolution of the methods employed).

Table 4. continued.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
4-Acid Digestion continued					
Co, Cobalt (ppm)	12.5	11.5	13.5	11.9	13.0
Cr, Chromium (ppm)	64	61	68	62	67
Cs, Caesium (ppm)	1.86	1.71	2.02	1.77	1.95
Cu, Copper (wt.%)	0.413	0.402	0.423	0.403	0.422
Dy, Dysprosium (ppm)	2.18	1.94	2.42	2.06	2.31
Er, Erbium (ppm)	1.13	0.92	1.34	1.09	1.18
Eu, Europium (ppm)	0.61	0.52	0.69	0.57	0.65
Fe, Iron (wt.%)	6.83	6.61	7.05	6.72	6.94
Ga, Gallium (ppm)	10.7	9.8	11.6	10.4	11.0
Gd, Gadolinium (ppm)	2.63	2.37	2.88	2.49	2.76
Hf, Hafnium (ppm)	1.33	1.18	1.47	1.27	1.38
Ho, Holmium (ppm)	0.40	0.35	0.46	0.38	0.42
In, Indium (ppm)	1.18	1.09	1.27	1.13	1.23
K, Potassium (wt.%)	1.62	1.58	1.66	1.59	1.65
La, Lanthanum (ppm)	15.9	14.3	17.4	15.2	16.5
Li, Lithium (ppm)	14.1	13.0	15.1	13.6	14.5
Lu, Lutetium (ppm)	0.17	0.14	0.20	IND	IND
Mg, Magnesium (wt.%)	0.388	0.373	0.403	0.378	0.397
Mn, Manganese (wt.%)	0.679	0.657	0.701	0.669	0.689
Mo, Molybdenum (ppm)	41.5	39.7	43.3	40.4	42.6
Na, Sodium (wt.%)	0.061	0.056	0.066	0.059	0.063
Nd, Neodymium (ppm)	15.8	14.5	17.1	15.3	16.4
Ni, Nickel (ppm)	101	97	105	98	103
P, Phosphorus (wt.%)	0.030	0.028	0.032	0.029	0.032
Pb, Lead (wt.%)	12.13	11.73	12.53	11.92	12.34
Pr, Praseodymium (ppm)	4.29	4.00	4.58	4.11	4.47
Rb, Rubidium (ppm)	73	68	78	71	75
Re, Rhenium (ppm)	0.096	0.076	0.115	0.086	0.105
S, Sulphur (wt.%)	14.78	14.28	15.28	14.45	15.10
Sb, Antimony (ppm)	224	207	242	216	233
Sc, Scandium (ppm)	5.31	4.85	5.77	5.08	5.54
Se, Selenium (ppm)	4.98	3.45	6.51	4.26	5.70
Sm, Samarium (ppm)	3.22	2.95	3.48	3.06	3.37
Sn, Tin (ppm)	3.61	3.16	4.05	3.42	3.79
Sr, Strontium (ppm)	101	97	106	98	104
Tb, Terbium (ppm)	0.37	0.34	0.41	0.35	0.40
Te, Tellurium (ppm)	0.82	0.65	0.99	0.60	1.04
Th, Thorium (ppm)	6.17	5.59	6.74	5.90	6.43
Ti, Titanium (wt.%)	0.106	0.095	0.118	0.103	0.109
Tl, Thallium (ppm)	17.8	16.8	18.8	17.5	18.2
Tm, Thulium (ppm)	0.18	0.15	0.21	IND	IND

SI unit equivalents: ppm (parts per million; 1×10^6) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

Note: intervals may appear asymmetric due to rounding.

IND = indeterminate (due to limited reading resolution of the methods employed).

Table 4. continued.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
4-Acid Digestion continued					
U, Uranium (ppm)	4.49	4.16	4.82	4.27	4.72
V, Vanadium (ppm)	67	64	70	65	69
W, Tungsten (ppm)	1.71	1.54	1.88	1.58	1.85
Y, Yttrium (ppm)	10.3	9.3	11.2	9.9	10.6
Yb, Ytterbium (ppm)	1.18	0.99	1.37	1.11	1.25
Zn, Zinc (wt.%)	17.45	17.10	17.79	17.24	17.66
Zr, Zirconium (ppm)	40.9	38.4	43.4	39.5	42.3
Aqua Regia Digestion					
Ag, Silver (ppm)	232	227	237	228	236
Al, Aluminium (wt.%)	0.508	0.462	0.553	0.495	0.520
As, Arsenic (ppm)	242	231	253	237	248
Be, Beryllium (ppm)	0.48	0.44	0.52	0.46	0.50
Bi, Bismuth (ppm)	44.1	42.2	46.0	42.8	45.4
Ca, Calcium (wt.%)	0.575	0.552	0.597	0.560	0.589
Cd, Cadmium (ppm)	369	354	385	362	376
Ce, Cerium (ppm)	27.0	23.4	30.6	26.0	27.9
Co, Cobalt (ppm)	10.3	9.0	11.5	9.9	10.6
Cr, Chromium (ppm)	24.1	22.7	25.4	23.0	25.2
Cs, Caesium (ppm)	0.70	0.64	0.77	0.68	0.73
Cu, Copper (wt.%)	0.422	0.408	0.436	0.414	0.430
Dy, Dysprosium (ppm)	1.10	0.87	1.32	1.05	1.15
Er, Erbium (ppm)	0.50	0.36	0.63	0.47	0.52
Eu, Europium (ppm)	0.38	0.35	0.41	0.36	0.40
Fe, Iron (wt.%)	6.78	6.56	6.99	6.64	6.92
Ga, Gallium (ppm)	4.14	3.68	4.61	3.92	4.36
Gd, Gadolinium (ppm)	1.57	1.19	1.95	1.49	1.66
Hf, Hafnium (ppm)	0.32	0.26	0.38	0.30	0.34
Hg, Mercury (ppm)	6.01	5.62	6.40	5.83	6.19
Ho, Holmium (ppm)	0.20	0.17	0.23	0.19	0.21
In, Indium (ppm)	1.15	1.06	1.25	1.10	1.20
K, Potassium (wt.%)	0.188	0.172	0.205	0.183	0.194
La, Lanthanum (ppm)	10.8	9.3	12.3	10.4	11.3
Li, Lithium (ppm)	5.36	4.37	6.35	5.19	5.53
Lu, Lutetium (ppm)	0.071	0.054	0.088	IND	IND
Mg, Magnesium (wt.%)	0.264	0.253	0.274	0.253	0.274
Mn, Manganese (wt.%)	0.664	0.637	0.690	0.652	0.675
Mo, Molybdenum (ppm)	41.1	39.3	42.9	40.1	42.1
Nd, Neodymium (ppm)	10.5	9.5	11.5	10.0	11.0
Ni, Nickel (ppm)	99	95	104	97	101
P, Phosphorus (wt.%)	0.029	0.027	0.031	0.028	0.030
Pb, Lead (wt.%)	12.19	11.93	12.45	11.94	12.43

SI unit equivalents: ppm (parts per million; 1×10^6) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

Note: intervals may appear asymmetric due to rounding.

IND = indeterminate (due to limited reading resolution of the methods employed).

Table 4. continued.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
Aqua Regia Digestion continued					
Pr, Praseodymium (ppm)	2.61	2.01	3.21	2.56	2.66
Rb, Rubidium (ppm)	11.4	9.5	13.2	10.8	11.9
Re, Rhenium (ppm)	0.11	0.09	0.12	IND	IND
S, Sulphur (wt.%)	14.92	14.36	15.48	14.61	15.22
Sb, Antimony (ppm)	200	189	211	195	205
Sc, Scandium (ppm)	1.27	1.05	1.48	IND	IND
Se, Selenium (ppm)	6.87	5.73	8.01	6.10	7.64
Sm, Samarium (ppm)	1.86	1.45	2.27	1.75	1.97
Sn, Tin (ppm)	2.52	2.22	2.83	2.39	2.66
Sr, Strontium (ppm)	21.2	19.6	22.8	20.3	22.1
Ta, Tantalum (ppm)	< 0.05	IND	IND	IND	IND
Tb, Terbium (ppm)	0.23	0.19	0.27	0.21	0.24
Te, Tellurium (ppm)	0.86	0.71	1.02	0.79	0.94
Th, Thorium (ppm)	5.07	4.73	5.41	4.91	5.23
Ti, Titanium (wt.%)	0.010	0.009	0.010	0.009	0.010
Tl, Thallium (ppm)	10.9	10.2	11.5	10.5	11.2
Tm, Thulium (ppm)	0.057	0.022	0.092	IND	IND
U, Uranium (ppm)	3.55	3.31	3.79	3.44	3.66
V, Vanadium (ppm)	16.2	14.5	18.0	15.4	17.0
W, Tungsten (ppm)	0.75	0.63	0.86	0.70	0.80
Y, Yttrium (ppm)	4.65	4.06	5.25	4.41	4.90
Yb, Ytterbium (ppm)	0.42	0.26	0.59	0.40	0.44
Zn, Zinc (wt.%)	17.49	17.16	17.83	17.17	17.82
Zr, Zirconium (ppm)	11.5	9.3	13.6	11.1	11.8

SI unit equivalents: ppm (parts per million; 1×10^6) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

Note: intervals may appear asymmetric due to rounding.

IND = indeterminate (due to limited reading resolution of the methods employed).

Homogeneity Evaluation

The tolerance limits (ISO 16269:2014) shown in Table 4 were determined using an analysis of precision errors method and are considered a conservative estimate of true homogeneity. The meaning of tolerance limits may be illustrated for Zn by 4-acid digestion, where 99% of the time ($1-\alpha=0.99$) at least 95% of subsamples ($p=0.95$) will have concentrations lying between 17.24 and 17.66 wt.%. Put more precisely, this means that if the same number of subsamples were taken and analysed in the same manner repeatedly, 99% of the tolerance intervals so constructed would cover at least 95% of the total population, and 1% of the tolerance intervals would cover less than 95% of the total population (ISO Guide 35). **Please note that tolerance limits pertain to the homogeneity of the CRM only and should not be used as control limits for laboratory performance.**

Based on the statistical analysis of the results of the inter-laboratory certification program it can be concluded that OREAS 317 is fit-for-purpose as a certified reference material (see 'Intended Use' below).

PARTICIPATING LABORATORIES

1. Actlabs, Ancaster, Ontario, Canada
2. AGAT Laboratories, Calgary, Alberta, Canada
3. AGAT Laboratories, Mississauga, Ontario, Canada
4. ALS, Brisbane, QLD, Australia
5. ALS, Lima, Peru
6. ALS, Loughrea, Galway, Ireland
7. ALS, Perth, WA, Australia
8. ALS, Vancouver, BC, Canada
9. American Assay Laboratories, Sparks, Nevada, USA
10. ARGETEST Mineral Processing, Ankara, Central Anatolia, Turkey
11. Bureau Veritas Commodities Canada Ltd, Vancouver, BC, Canada
12. Bureau Veritas Geoanalytical, Adelaide, SA, Australia
13. Bureau Veritas Geoanalytical, Perth, WA, Australia
14. ESAN Balya, Balya, Turkey
15. ESAN Istanbul, Istanbul, Turkey
16. Intertek Genalysis, Perth, WA, Australia
17. Intertek Testing Services Philippines, Cupang, Muntinlupa, Philippines
18. MinAnalytical Services, Perth, WA, Australia
19. MSALABS, Vancouver, BC, Canada
20. PT Geoservices Ltd, Cikarang, Jakarta Raya, Indonesia
21. PT Intertek Utama Services, Jakarta Timur, DKI Jakarta, Indonesia
22. Saskatchewan Research Council, Saskatoon, Saskatchewan, Canada
23. SGS, Randfontein, Gauteng, South Africa
24. SGS Australia Mineral Services, Perth, WA, Australia
25. SGS Geosol Laboratorios Ltda, Vespasiano, Minas Gerais, Brazil
26. Shiva Analyticals Ltd, Bangalore North, Karnataka, India

Please note: To preserve anonymity, the above numbered alphabetical list of participating laboratories does not correspond with the Lab ID numbering on the scatter plots below.

PREPARER

Certified reference material OREAS 317 was prepared and certified by:



ORE Research & Exploration Pty Ltd
37A Hosie Street
Bayswater North VIC 3153
AUSTRALIA

Tel: +613-9729 0333
Fax: +613-9729 8338
Web: www.oreas.com
Email: info@oreas.com

Figure 1. Ag by 4-Acid Digestion in OREAS 317

SPC.1566.RR1.OREAS 317.2.4-Acid.Ag.Lab.220329.194435.SN

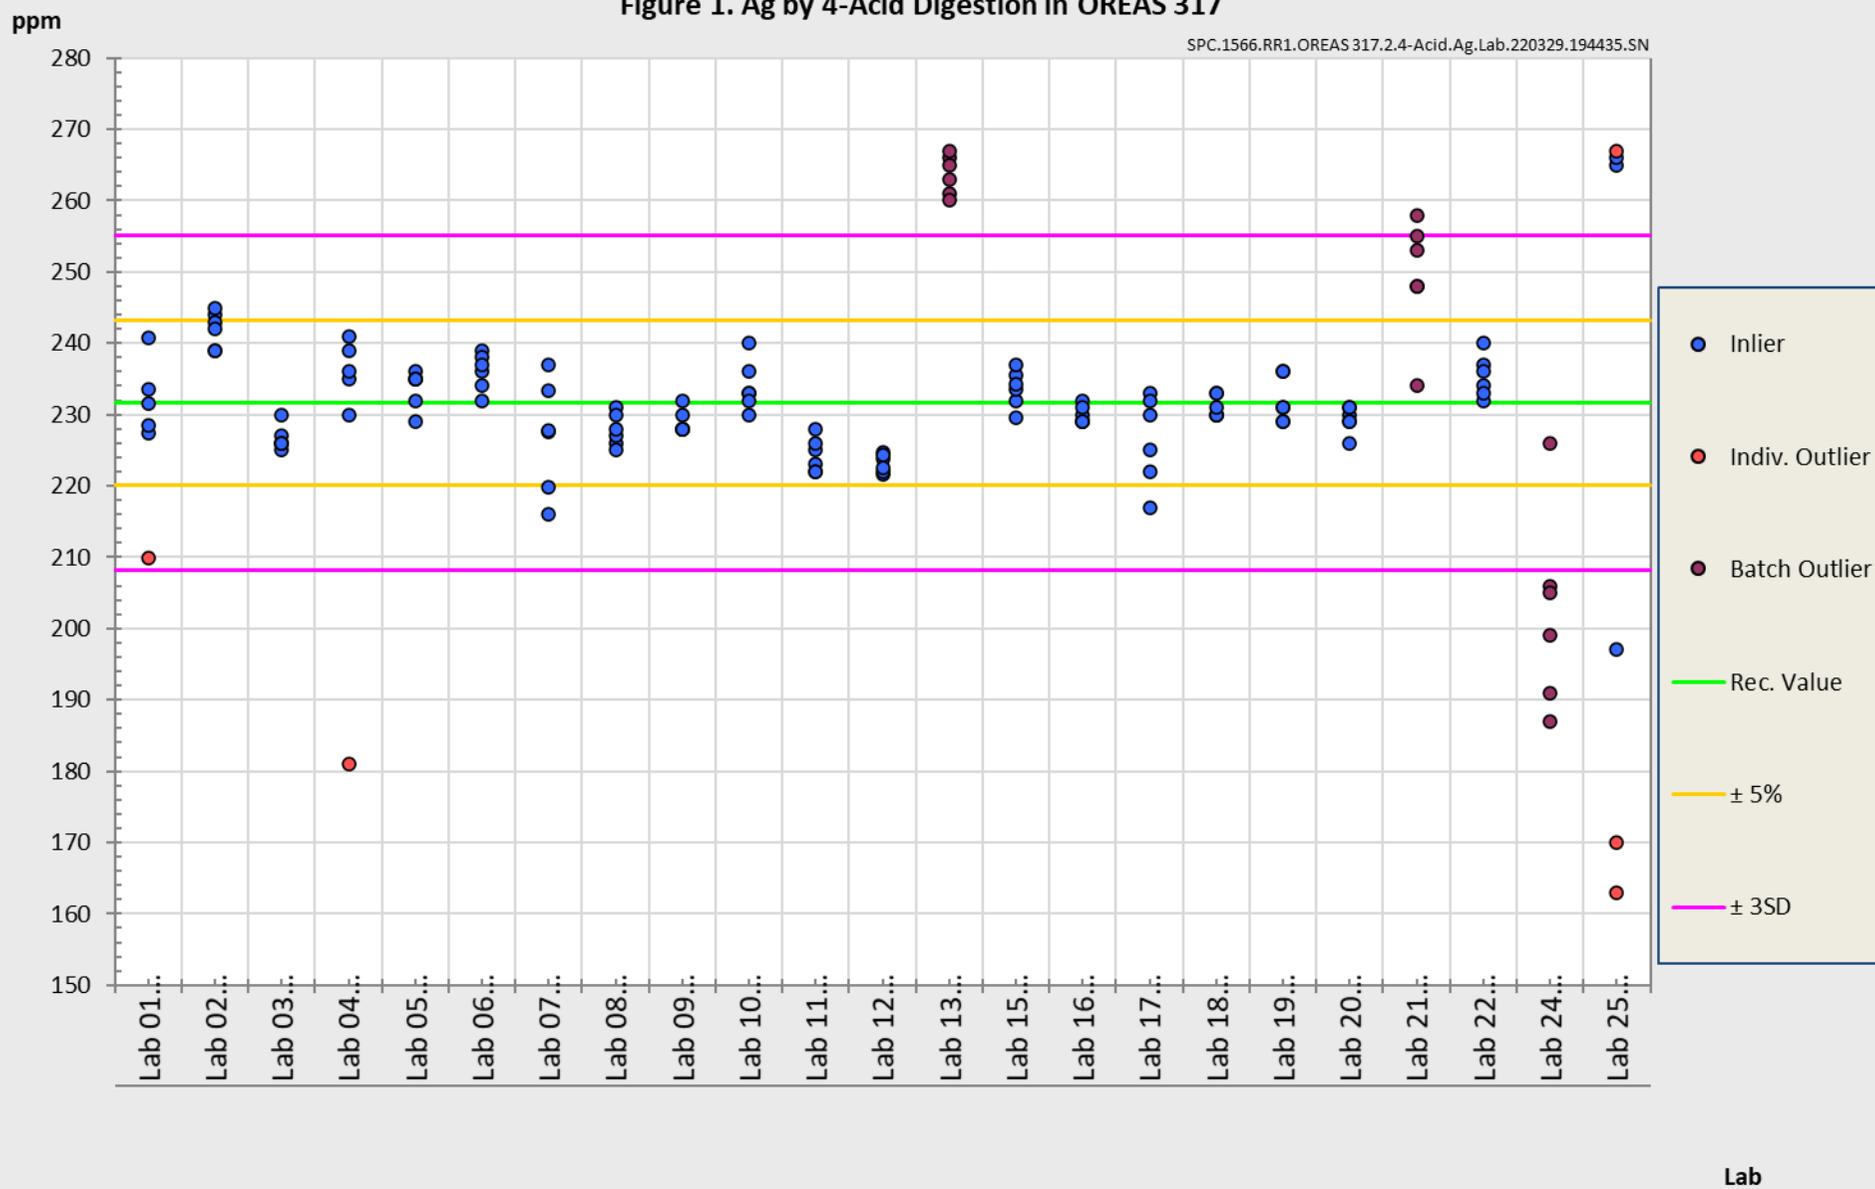


Figure 2. Pb by 4-Acid Digestion in OREAS 317

SPC.1566.RR1.OREAS 317.2.4-Acid.Pb.Lab.220330.233839.SS


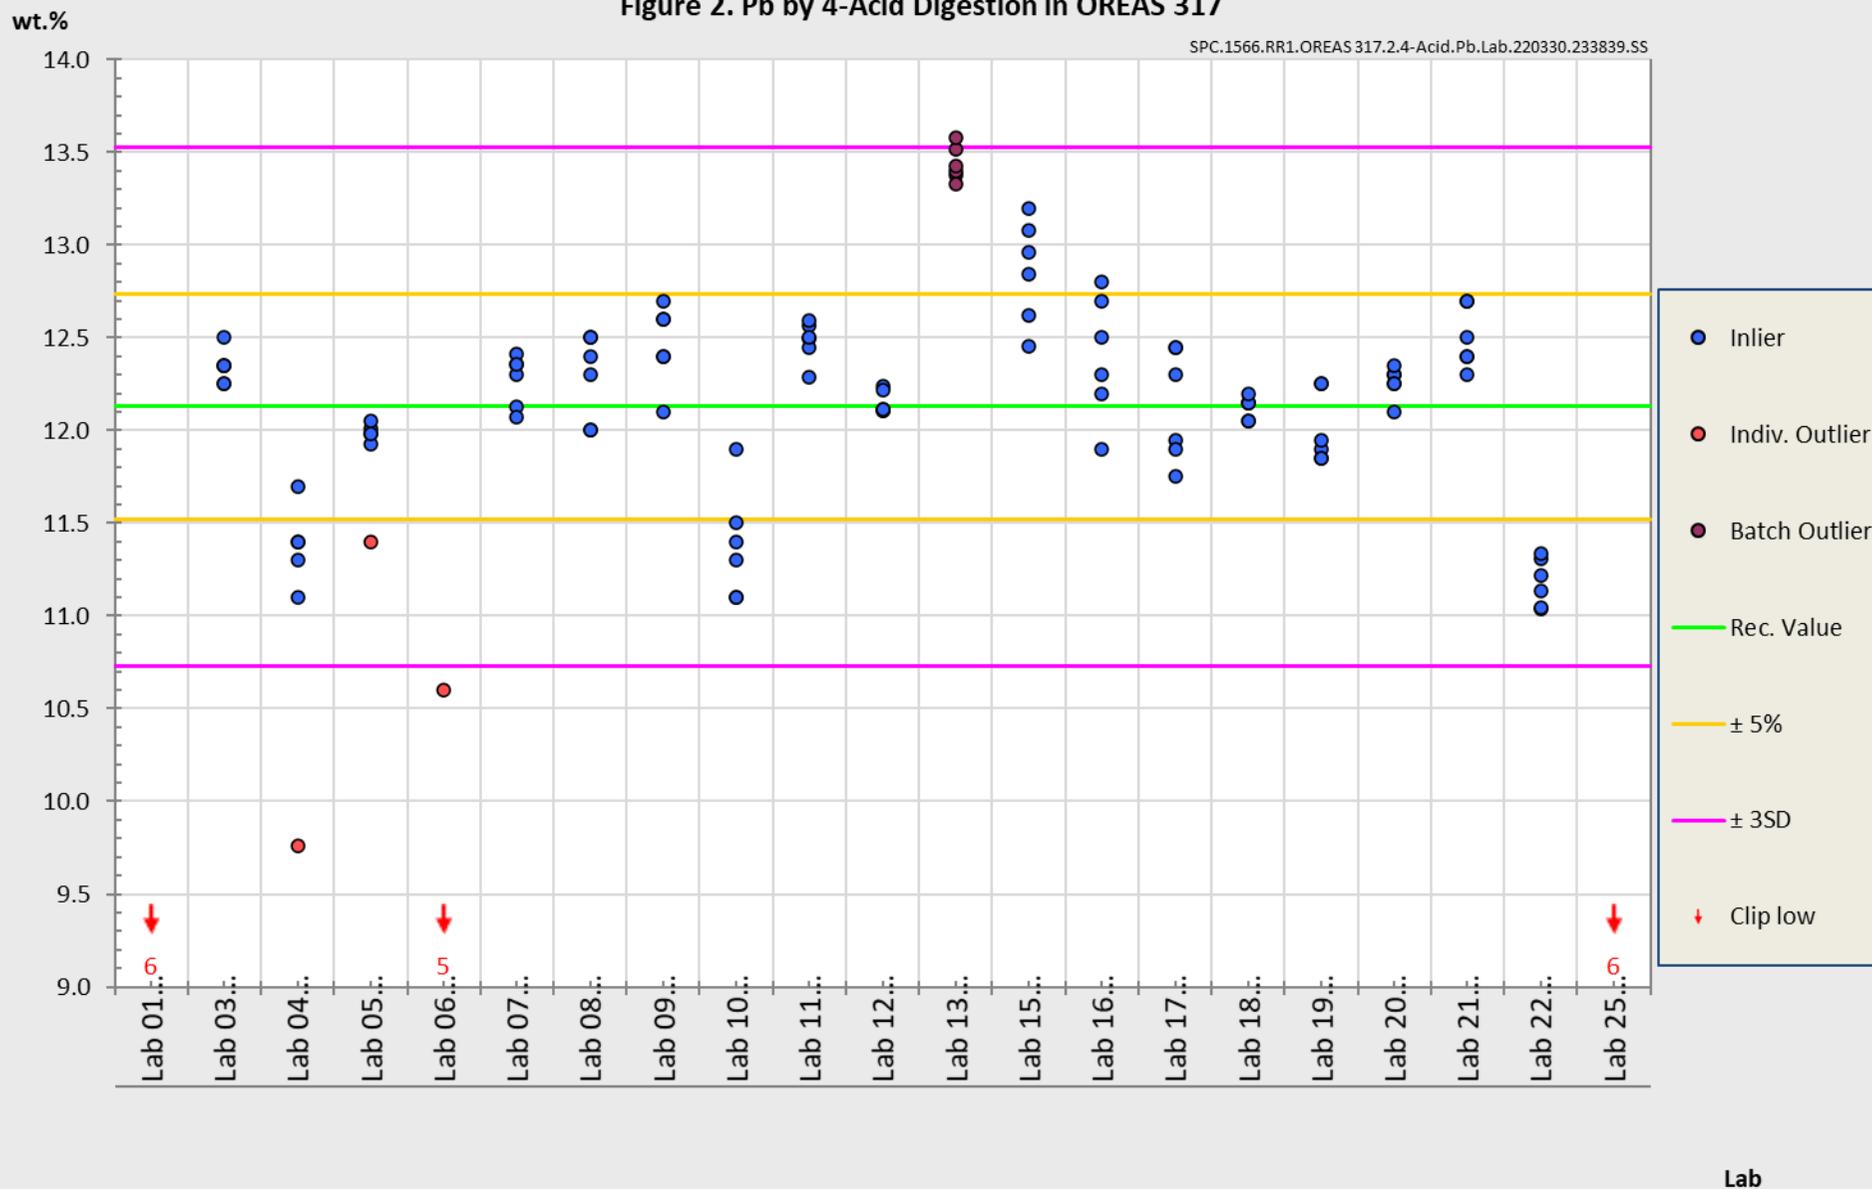


Figure 3. Zn by 4-Acid Digestion in OREAS 317

SPC.1566.RR1.OREAS 317.2.4-Acid.Zn.Lab.220329.194618.SN

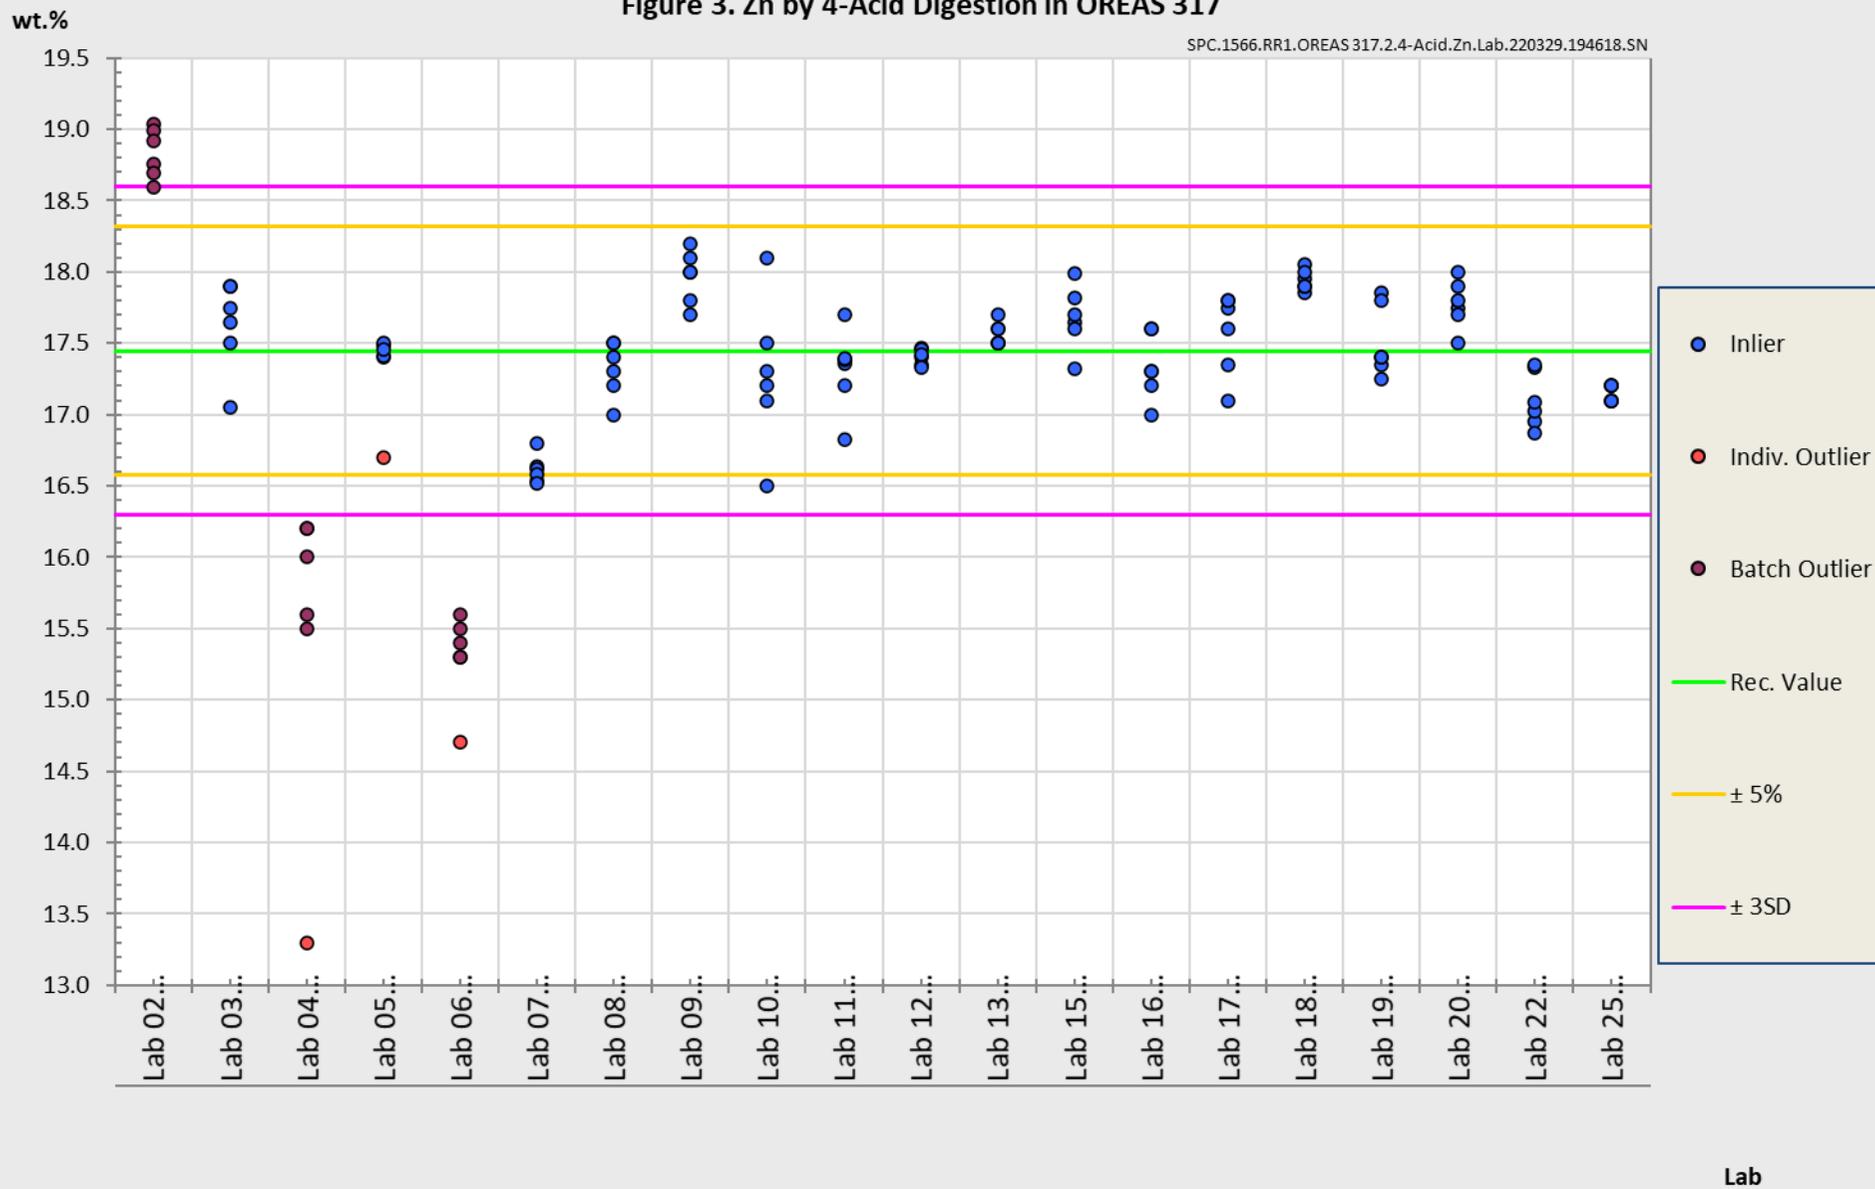

METROLOGICAL TRACEABILITY

The analytical samples were selected in a manner representative of the entire batch of the prepared CRM. This 'representivity' was maintained in each submitted laboratory sample batch and ensures the user that the data is traceable from sample selection through to the analytical results that underlie the consensus values. Each analytical data set has been validated by its assayer through the inclusion of internal reference materials and QC checks during analysis.

The laboratories were chosen on the basis of their competence (from past performance in inter-laboratory programs undertaken by ORE Pty Ltd) for a particular analytical method, analyte or analyte suite and sample matrix. Most of these laboratories have and maintain ISO 17025 accreditation. The certified values presented in this report are calculated from the means of accepted data following robust statistical treatment, as detailed in this report.

Guide ISO/TR 16476:2016, section 5.3.1 describes metrological traceability in reference materials as it pertains to the transformation of the measurand. In this section it states, *"Although the determination of the property value itself can be made traceable to appropriate units through, for example, calibration of the measurement equipment used, steps like the transformation of the sample from one physical (chemical) state to another cannot. Such transformations may only be compared with a reference (when available), or among themselves. For some transformations, reference methods have been defined and may be used in certification projects to evaluate the uncertainty associated with such a transformation. In other cases, only a comparison among different laboratories using the same procedure is possible. In this case, it is impossible to demonstrate absence of method bias; therefore, the result is an operationally defined measurand (ISO Guide 35:2017, 9.2.4c)."* Certification takes place on the basis of agreement among operationally defined, independent measurement results.

COMMUTABILITY

The measurements of the results that underlie the certified values contained in this report were undertaken by methods involving pre-treatment (digestion/fusion) of the sample. This served to reduce the sample to a simple and well understood form permitting calibration using simple solutions of the CRM. Due to these methods being well understood and highly effective, commutability is not an issue for this CRM. Being matrix-matched, OREAS 317 will display similar behaviour in the relevant measurement process to the routine field samples for which OREAS 317 is designated to monitor. To maintain commutability, care should be taken to always ensure 'matrix matching' as close as practically achievable. The matrix and mineralisation style of the CRM is described in the 'Source Material' section and users should select appropriate CRMs matching these attributes to their metallurgical plant samples.

INTENDED USE

OREAS 317 is intended to cover all activities needed to produce a measurement result. This includes extraction, possible separation steps and the actual measurement process (the signal producing step). OREAS 317 may be used to calibrate the entire procedure by producing a pure substance CRM transformed into a calibration solution.

OREAS 317 is intended for the following uses:

- For the monitoring of laboratory performance in the analysis of analytes reported in Table 1 in sulphide concentrate samples;
- For the verification of analytical methods for analytes reported in Table 1;
- For the calibration of instruments used in the determination of the concentration of analytes reported in Table 1.

PERIOD OF VALIDITY & STORAGE INSTRUCTIONS

The certification of OREAS 317 remains valid, within the specified measurement uncertainties, until January 2037, provided the CRM is handled and stored in accordance with the instructions given below. This certification is nullified if the CRM is any way changed or contaminated.

Store in a clean and cool dry place away from direct sunlight.

Long-term stability will be monitored at appropriate intervals and purchasers notified if any changes are observed. The period of validity may well be indefinite and will be reassessed prior to expiry with the aim of extending the validity if possible.

Single-use sachets

OREAS 317 is sulphide rich (15.2 wt.% S) and is packaged in single-use sachets sealed under nitrogen. Following analysis, it is the manufacturer's expectation that any remaining material is discarded. It is the user's responsibility to prevent contamination and avoid prolonged exposure of the sample to the atmosphere prior to analysis.

INSTRUCTIONS FOR HANDLING & CORRECT USE

Pre-homogenisation of the CRM prior to subsampling and analysis is not necessary as there is no particle segregation under transport [12].

Fine powders pose a risk to eyes and lungs and therefore standard precautions including the use of safety glasses and dust masks are advised. Sulphur is a known transitory upper respiratory irritant. Close exposure may cause coughing or throat irritation.

As per routine analysis at commercial laboratories, the certified values derived by oxidising fusion with XRF finish are on a dry sample basis.

Analytes by all other methods refer to the concentration levels in the packaged state. There is no need for drying prior to weighing and analysis for these methods.

Minimum sample size

As a practical guide, the minimum mass of sample used should match the typical mass that the laboratories used in the interlaboratory (round robin) certification program. This means that different sample masses should be used depending on the operationally defined methodology.

- Oxidising fusion with X-ray fluorescence finish: $\geq 0.2\text{g}$;
- Loss on Ignition (LOI) at 1000°C : $\geq 1\text{g}$;

- Total C and S by IR induction furnace: $\geq 0.1\text{g}$;
- Peroxide or borate fusion with ICP-OES and/or MS finish: $\geq 0.1\text{g}$;
- 4-acid digestion with ICP-OES and/or MS finish: $\geq 0.25\text{g}$;
- Aqua regia digestion with ICP-OES and/or MS finish: $\geq 0.5\text{g}$.

QC monitoring using multiples of the Standard Deviation (SD)

In the application of SD's in monitoring performance it is important to note that not all laboratories function at the same level of proficiency and that different methods in use at a particular laboratory have differing levels of precision. Each laboratory has its own inherent SD (for a specific concentration level and analyte-method pair) based on the analytical process and this SD is not directly related to the round robin program.

The majority of data generated in the round robin program was produced by a selection of world class laboratories. The SD's thus generated are more constrained than those that would be produced across a randomly selected group of laboratories. To produce more generally achievable SD's the 'pooled' SD's provided in this report include inter-laboratory bias. This 'one size fits all' approach may require revision at the discretion of the QC manager concerned following careful scrutiny of QC control charts.

The performance gates shown in Table 1 are intended only to be used as a first principle guide as to what a laboratory may be able to achieve. Over a period of time monitoring your own laboratory's data for this CRM, SD's should be calculated directly from your own laboratory's process. This will enable you to establish more specific performance gates that are fit for purpose for your application as well as the ability to monitor bias. If your long-term trend analysis shows an average value that is within the 95% expanded uncertainty interval then generally there is no cause for concern in regard to bias.

For use with the aqua regia digestion method

It is important to note that in the analytical industry there is no standardisation of the aqua regia digestion process. Aqua regia is a partial empirical digest and differences in recoveries for various analytes are commonplace. These are caused by variations in the digest conditions which can include the ratio of nitric to hydrochloric acids, acid strength, temperatures, leach times and secondary digestions. Recoveries for sulphide-hosted base metal sulphides approach total values, however other analytes, in particular the lithophile elements, show greater sensitivity to method parameters. This can result in lack of consensus in an inter-laboratory certification program for these elements.

The approach applied here is to report certified values in those instances where reasonable agreement exists amongst a majority of participating laboratories. The results from specific laboratories may differ significantly from the certified values, but will, nonetheless, be valid and reproducible in the context of the specifics of the aqua regia method in use. Users of this reference material should, therefore, be mindful of this limitation when applying the certified values in a quality control program.

DOCUMENT HISTORY

Revision No.	Date	Changes applied
0	30 th March, 2022	First publication.

QMS CERTIFICATION

ORE Pty Ltd is ISO 9001:2015 certified by Lloyd's Register Quality Assurance Ltd for its quality management system including development, manufacturing, certification and supply of CRMs.



CERTIFYING OFFICER

A handwritten signature in blue ink, appearing to read 'S. Hamlyn'.

30th March, 2022

Craig Hamlyn (B.Sc. Hons - Geology), Technical Manager - ORE P/L

LEGAL NOTICE

Ore Research & Exploration Pty Ltd has prepared and statistically evaluated the property values of this reference material to the best of its ability. The Purchaser by receipt hereof releases and indemnifies Ore Research & Exploration Pty Ltd from and against all liability and costs arising from the use of this material and information.

REFERENCES

- [1] Govett, G.J.S. (1983). Handbook of Exploration Geochemistry, Volume 2: Statistics and Data Analysis in Geochemical Prospecting (Variations of accuracy and precision).
- [2] ISO Guide 30:2015. Terms and definitions used in connection with reference materials.
- [3] ISO Guide 31:2015. Reference materials – Contents of certificates and labels.
- [4] ISO Guide 35:2017. Certification of reference materials - General and statistical principals.
- [5] JCGM 100:2008; Evaluation of Measurement Data — Guide to the Expression of Uncertainty in Measurement (GUM 1995 with Minor Corrections); Joint Committee for Guides in Metrology (JCGM) (2008); available at www.bipm.org/utils/common/documents/jcgm/JCGM_100_2008_E.pdf (accessed Nov 2021), (also known as ISO Guide 98-3:2008. Guide to the expression of uncertainty in measurement).
- [6] ISO 16269:2014. Statistical interpretation of data – Part 6: Determination of statistical tolerance intervals.
- [7] ISO/TR 16476:2016, Reference Materials – Establishing and expressing metrological traceability of quantity values assigned to reference materials.
- [8] ISO 17025:2005, General requirements for the competence of testing and calibration laboratories.

- [9] ISO Guide 17034:2016. General requirements for the competence of reference material producers.
- [10] Munsell Rock Color Book (2014). Rock-Color Chart Committee, Geological Society of America (GSA), Minnesota (USA).
- [11] OREAS-BUP-70-09-11: Statistical Analysis - OREAS Evaluation Method.
- [12] OREAS-TN-04-1498: Stability under transport; an experimental study of OREAS CRMs.
- [13] OREAS-TN-05-1674: Long-term storage stability; an experimental study of OREAS CRMs.
- [14] Thompson, A.; Taylor, B.N.; Guide for the Use of the International System of Units (SI); NIST Special Publication 811; U.S. Government Printing Office: Washington, DC (2008); available at: <https://physics.nist.gov/cuu/pdf/sp811.pdf> (accessed Nov 2021).
- [15] Van der Veen AMH and Pauwels, J. (2001), Accred Qual Assur 6: 290-294.