




ORE RESEARCH & EXPLORATION P/L ABN 28 006 859 856
37A Hosie Street · Bayswater North · VIC 3153 · AUSTRALIA
☎ 61 3 9729 0333 ☎ 61 3 9729 8338
📧 info@ore.com.au 🌐 www.oreas.com

CERTIFICATE OF ANALYSIS FOR

CERTIFIED REFERENCE MATERIAL

OREAS 920b

Copper-bearing siltstone (Cobar, NSW, Australia)



COA-1652-OREAS920b-R1
BUP-70-10-01 Ver:2.0

19-Feb-2024

Table 1. Certified Values, Uncertainty & Tolerance Intervals for OREAS 920b.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
4-Acid Digestion					
Ag, Silver (ppm)	0.320	0.297	0.343	0.296	0.345
Al, Aluminium (wt.%)	6.79	6.59	7.00	6.65	6.94
As, Arsenic (ppm)	113	108	118	110	117
Ba, Barium (ppm)	2105	2023	2188	2056	2155
Be, Beryllium (ppm)	2.59	2.44	2.74	2.51	2.67
Bi, Bismuth (ppm)	0.79	0.75	0.83	0.77	0.82
Ca, Calcium (wt.%)	0.030	0.030	0.030	0.029	0.031
Cd, Cadmium (ppm)	0.042	0.024	0.060	IND	IND
Ce, Cerium (ppm)	90	86	94	87	93
Co, Cobalt (ppm)	1.63	1.55	1.71	1.54	1.72
Cr, Chromium (ppm)	87	81	93	84	90
Cs, Caesium (ppm)	4.43	4.27	4.58	4.31	4.54
Cu, Copper (ppm)	116	112	120	113	119
Dy, Dysprosium (ppm)	3.62	3.14	4.10	3.42	3.82
Er, Erbium (ppm)	1.72	1.60	1.85	1.62	1.83
Eu, Europium (ppm)	1.29	1.12	1.46	1.24	1.34
Fe, Iron (wt.%)	3.03	2.93	3.12	2.96	3.09
Ga, Gallium (ppm)	20.3	19.4	21.3	19.7	20.9
Gd, Gadolinium (ppm)	5.49	4.73	6.24	5.26	5.71
Hf, Hafnium (ppm)	2.32	2.19	2.45	2.22	2.42
Ho, Holmium (ppm)	0.61	0.53	0.69	0.58	0.65
In, Indium (ppm)	0.075	0.069	0.082	0.069	0.082
K, Potassium (wt.%)	2.71	2.62	2.80	2.62	2.80
La, Lanthanum (ppm)	43.5	41.8	45.1	42.2	44.7
Li, Lithium (ppm)	21.3	20.4	22.3	20.8	21.9
Lu, Lutetium (ppm)	0.26	0.24	0.29	0.25	0.28
Mg, Magnesium (wt.%)	0.377	0.363	0.390	0.367	0.386
Mn, Manganese (wt.%)	0.007	0.007	0.007	0.007	0.007
Mo, Molybdenum (ppm)	2.93	2.79	3.07	2.81	3.05
Na, Sodium (wt.%)	0.098	0.089	0.106	0.094	0.101
Nb, Niobium (ppm)	5.04	4.15	5.94	4.58	5.51
Nd, Neodymium (ppm)	36.2	32.6	39.7	34.7	37.6
Ni, Nickel (ppm)	12.1	11.6	12.5	11.6	12.5
P, Phosphorus (wt.%)	0.032	0.031	0.033	0.031	0.033
Pb, Lead (ppm)	26.4	25.4	27.4	25.5	27.3
Pr, Praseodymium (ppm)	10.1	8.8	11.4	9.7	10.4
Rb, Rubidium (ppm)	156	149	162	151	160

SI unit equivalents: ppm (parts per million; $1 \times 10^{-6} \equiv \text{mg/kg}$; wt.% (weight per cent) $\equiv \%$ (mass fraction).

Note: intervals may appear asymmetric due to rounding; IND = indeterminate (due to limited reading resolution of the methods employed).

Table 1 continued.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
4-Acid Digestion continued					
Re, Rhenium (ppm)	< 0.002	IND	IND	IND	IND
S, Sulphur (wt.%)	0.029	0.028	0.031	0.027	0.031
Sb, Antimony (ppm)	3.97	3.78	4.17	3.80	4.15
Sc, Scandium (ppm)	12.5	12.0	13.0	12.0	13.0
Se, Selenium (ppm)	2.37	1.71	3.02	2.09	2.64
Sm, Samarium (ppm)	7.09	6.43	7.76	6.74	7.45
Sn, Tin (ppm)	3.91	3.72	4.11	3.72	4.11
Sr, Strontium (ppm)	57	55	59	55	58
Ta, Tantalum (ppm)	0.40	0.31	0.49	0.36	0.45
Tb, Terbium (ppm)	0.71	0.62	0.79	0.68	0.73
Te, Tellurium (ppm)	0.088	0.067	0.109	IND	IND
Th, Thorium (ppm)	15.5	14.7	16.3	15.1	15.9
Ti, Titanium (wt.%)	0.226	0.209	0.243	0.215	0.237
Tl, Thallium (ppm)	0.85	0.81	0.89	0.82	0.88
Tm, Thulium (ppm)	0.25	0.22	0.29	0.23	0.28
U, Uranium (ppm)	4.06	3.88	4.25	3.93	4.20
V, Vanadium (ppm)	166	160	172	160	172
W, Tungsten (ppm)	1.91	1.71	2.10	1.77	2.04
Y, Yttrium (ppm)	15.5	14.2	16.7	14.8	16.1
Yb, Ytterbium (ppm)	1.61	1.46	1.77	1.53	1.70
Zn, Zinc (ppm)	57	55	59	55	58
Zr, Zirconium (ppm)	80	76	83	76	84
Aqua Regia Digestion					
Ag, Silver (ppm)	0.174	0.163	0.186	0.157	0.192
Al, Aluminium (wt.%)	0.749	0.707	0.790	0.727	0.771
As, Arsenic (ppm)	111	107	115	108	114
Au, Gold (ppm)	0.019	0.015	0.024	0.016	0.023
B, Boron (ppm)	< 10	IND	IND	IND	IND
Ba, Barium (ppm)	190	174	206	184	196
Be, Beryllium (ppm)	0.52	0.46	0.58	0.50	0.54
Bi, Bismuth (ppm)	0.59	0.55	0.63	0.56	0.62
Ca, Calcium (wt.%)	0.023	0.018	0.027	0.022	0.024
Cd, Cadmium (ppm)	0.033	0.022	0.045	IND	IND
Ce, Cerium (ppm)	79	75	82	76	81
Co, Cobalt (ppm)	1.47	1.37	1.57	IND	IND
Cr, Chromium (ppm)	23.1	22.1	24.0	22.2	23.9
Cs, Caesium (ppm)	1.08	0.99	1.18	1.04	1.13

SI unit equivalents: ppm (parts per million; $1 \times 10^{-6} \equiv \text{mg/kg}$; wt.% (weight per cent) \equiv % (mass fraction).

Note: intervals may appear asymmetric due to rounding; IND = indeterminate (due to limited reading resolution of the methods employed). For practical purposes the 95% Expanded Uncertainty can be set between zero and a two times multiple of the upper bound/non-detect limit value).

Table 1 continued.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
Aqua Regia Digestion continued					
Cu, Copper (ppm)	115	111	119	112	118
Fe, Iron (wt.%)	2.77	2.68	2.85	2.70	2.83
Ga, Gallium (ppm)	2.64	2.37	2.91	2.52	2.75
Hf, Hafnium (ppm)	0.35	0.31	0.39	0.33	0.37
In, Indium (ppm)	0.024	0.019	0.030	0.022	0.027
K, Potassium (wt.%)	0.263	0.243	0.284	0.252	0.274
La, Lanthanum (ppm)	33.0	31.7	34.4	32.0	34.1
Li, Lithium (ppm)	2.90	2.57	3.23	2.76	3.04
Lu, Lutetium (ppm)	0.11	0.10	0.13	IND	IND
Mg, Magnesium (wt.%)	0.088	0.081	0.096	0.085	0.092
Mn, Manganese (wt.%)	0.005	0.005	0.005	0.005	0.005
Mo, Molybdenum (ppm)	2.75	2.60	2.89	2.63	2.87
Nb, Niobium (ppm)	0.054	0.044	0.064	IND	IND
Ni, Nickel (ppm)	9.00	8.57	9.42	8.70	9.29
P, Phosphorus (wt.%)	0.026	0.025	0.028	0.026	0.027
Pb, Lead (ppm)	16.6	15.5	17.8	16.0	17.3
Rb, Rubidium (ppm)	15.6	14.5	16.8	14.9	16.4
Re, Rhenium (ppm)	< 0.001	IND	IND	IND	IND
S, Sulphur (wt.%)	0.026	0.022	0.029	0.024	0.028
Sb, Antimony (ppm)	2.54	2.29	2.78	2.44	2.63
Sc, Scandium (ppm)	1.57	1.43	1.71	IND	IND
Se, Selenium (ppm)	2.24	2.04	2.44	2.07	2.41
Sn, Tin (ppm)	0.59	0.50	0.67	0.43	0.74
Sr, Strontium (ppm)	14.0	12.5	15.6	13.4	14.6
Ta, Tantalum (ppm)	< 0.01	IND	IND	IND	IND
Tb, Terbium (ppm)	0.50	0.46	0.54	0.47	0.53
Te, Tellurium (ppm)	0.071	0.055	0.088	IND	IND
Th, Thorium (ppm)	10.4	9.9	10.9	10.2	10.7
Ti, Titanium (wt.%)	0.011	0.009	0.012	0.010	0.012
Tl, Thallium (ppm)	0.10	0.09	0.11	IND	IND
U, Uranium (ppm)	2.39	2.29	2.48	2.33	2.45
V, Vanadium (ppm)	19.3	18.2	20.4	18.4	20.2
W, Tungsten (ppm)	0.11	0.09	0.13	IND	IND
Y, Yttrium (ppm)	7.25	6.85	7.66	7.02	7.48
Zn, Zinc (ppm)	47.5	46.1	49.0	46.2	48.9
Zr, Zirconium (ppm)	12.2	11.2	13.2	11.7	12.6

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

Note: intervals may appear asymmetric due to rounding; IND = indeterminate (due to limited reading resolution of the methods employed. For practical purposes the 95% Expanded Uncertainty can be set between zero and a two times multiple of the upper bound/non-detect limit value).

Table 1 continued.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
Borate / Peroxide Fusion ICP					
Ag, Silver (ppm)	< 5	IND	IND	IND	IND
Al, Aluminium (wt.%)	6.98	6.82	7.14	6.85	7.11
As, Arsenic (ppm)	110	100	119	105	114
B, Boron (ppm)	138	124	152	131	145
Ba, Barium (ppm)	2114	2025	2204	2058	2171
Be, Beryllium (ppm)	2.48	2.03	2.93	2.18	2.79
Bi, Bismuth (ppm)	0.87	0.72	1.03	IND	IND
Ca, Calcium (wt.%)	< 0.1	IND	IND	IND	IND
Ce, Cerium (ppm)	92	85	99	88	96
Co, Cobalt (ppm)	1.76	1.44	2.07	IND	IND
Cr, Chromium (ppm)	109	95	122	102	116
Cs, Caesium (ppm)	4.52	4.12	4.93	4.22	4.82
Cu, Copper (ppm)	119	104	133	112	125
Dy, Dysprosium (ppm)	4.96	4.43	5.49	4.61	5.31
Er, Erbium (ppm)	2.79	2.56	3.03	2.62	2.96
Eu, Europium (ppm)	1.31	1.09	1.52	1.21	1.40
Fe, Iron (wt.%)	3.03	2.96	3.10	2.98	3.08
Ga, Gallium (ppm)	20.5	18.7	22.2	19.3	21.7
Gd, Gadolinium (ppm)	5.81	5.17	6.45	5.53	6.09
Ge, Germanium (ppm)	2.33	1.90	2.76	1.91	2.74
Ho, Holmium (ppm)	0.97	0.87	1.08	0.89	1.05
In, Indium (ppm)	< 0.2	IND	IND	IND	IND
K, Potassium (wt.%)	2.76	2.66	2.87	2.70	2.82
La, Lanthanum (ppm)	43.6	40.6	46.6	41.9	45.3
Li, Lithium (ppm)	21.7	18.8	24.7	20.0	23.5
Lu, Lutetium (ppm)	0.41	0.36	0.45	0.37	0.45
Mg, Magnesium (wt.%)	0.387	0.372	0.402	0.373	0.402
Mn, Manganese (wt.%)	0.008	0.007	0.008	0.007	0.008
Mo, Molybdenum (ppm)	3.37	2.69	4.06	IND	IND
Nb, Niobium (ppm)	12.2	10.9	13.4	11.0	13.3
Nd, Neodymium (ppm)	36.7	33.5	39.8	34.9	38.4
P, Phosphorus (wt.%)	0.032	0.024	0.040	IND	IND
Pb, Lead (ppm)	30.3	26.6	34.0	28.3	32.3
Pr, Praseodymium (ppm)	9.90	9.06	10.74	9.42	10.37
Rb, Rubidium (ppm)	154	145	162	149	159
Re, Rhenium (ppm)	< 0.1	IND	IND	IND	IND
S, Sulphur (wt.%)	0.035	0.019	0.050	IND	IND

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

Note: intervals may appear asymmetric due to rounding; IND = indeterminate (due to limited reading resolution of the methods employed. For practical purposes the 95% Expanded Uncertainty can be set between zero and a two times multiple of the upper bound/non-detect limit value).

Table 1 continued.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
Borate / Peroxide Fusion ICP continued					
Sb, Antimony (ppm)	4.10	3.71	4.49	3.87	4.34
Sc, Scandium (ppm)	12.0	10.8	13.2	IND	IND
Si, Silicon (wt.%)	35.16	34.26	36.06	34.68	35.64
Sm, Samarium (ppm)	6.75	6.21	7.29	6.31	7.19
Sr, Strontium (ppm)	60	55	66	58	63
Ta, Tantalum (ppm)	0.85	0.65	1.05	0.59	1.11
Tb, Terbium (ppm)	0.83	0.74	0.93	0.79	0.88
Te, Tellurium (ppm)	< 1	IND	IND	IND	IND
Th, Thorium (ppm)	14.7	13.6	15.7	14.0	15.4
Ti, Titanium (wt.%)	0.330	0.317	0.344	0.323	0.337
Tl, Thallium (ppm)	0.88	0.79	0.96	0.82	0.94
Tm, Thulium (ppm)	0.42	0.38	0.46	0.39	0.45
U, Uranium (ppm)	4.43	4.05	4.81	4.22	4.64
V, Vanadium (ppm)	176	169	183	172	181
W, Tungsten (ppm)	3.01	2.03	3.99	2.59	3.43
Y, Yttrium (ppm)	27.5	25.7	29.3	26.4	28.5
Yb, Ytterbium (ppm)	2.75	2.50	3.00	2.59	2.92
Zn, Zinc (ppm)	61	53	69	56	66

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

Note: intervals may appear asymmetric due to rounding; IND = indeterminate (due to limited reading resolution of the methods employed. For practical purposes the 95% Expanded Uncertainty can be set between zero and a two times multiple of the upper bound/non-detect limit value).

Table 2. Indicative Values for OREAS 920b.

Constituent	Unit	Value	Constituent	Unit	Value	Constituent	Unit	Value
4-Acid Digestion								
B	ppm	20.2	Ge	ppm	0.22	Hg	ppm	0.026
Aqua Regia Digestion								
Dy	ppm	2.24	Hg	ppm	0.015	Pr	ppm	8.09
Er	ppm	0.87	Ho	ppm	0.36	Pt	ppb	< 5
Eu	ppm	0.98	Na	wt.%	0.010	Sm	ppm	5.35
Gd	ppm	4.14	Nd	ppm	29.7	Tm	ppm	0.10
Ge	ppm	0.10	Pd	ppb	66.7	Yb	ppm	0.72
Borate Fusion XRF								
Cd	ppm	< 0.8	Ni	ppm	21.0	Zr	ppm	101
Hf	ppm	3.05	Se	ppm	1.99			
Na	wt.%	0.111	Sn	ppm	8.65			
Thermogravimetry								
LOI ¹⁰⁰⁰	wt.%	3.67						
Infrared Combustion								
C	wt.%	0.784	S	wt.%	0.026			

SI unit equivalents: ppb (parts per billion; 1×10^{-9}) \equiv μ g/kg; ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction). Note: the number of significant figures reported is not a reflection of the level of certainty of stated values. They are instead an artefact of ORE's in-house CRM-specific LIMS.

TABLE OF CONTENTS

INTRODUCTION	8
SOURCE MATERIAL.....	8
COMMINUTION AND HOMOGENISATION PROCEDURES	8
PHYSICAL PROPERTIES	9
ANALYTICAL PROGRAM.....	9
STATISTICAL ANALYSIS.....	9
PERFORMANCE GATES	10
Homogeneity Evaluation	15
PARTICIPATING LABORATORIES.....	17
PREPARER AND SUPPLIER.....	17
METROLOGICAL TRACEABILITY	17
COMMUTABILITY	18
INTENDED USE	19
PERIOD OF VALIDITY & STORAGE INSTRUCTIONS.....	19
INSTRUCTIONS FOR HANDLING & CORRECT USE.....	20
LEGAL NOTICE.....	21
DOCUMENT HISTORY	21
QMS CERTIFICATION	21
CERTIFYING OFFICER.....	22
REFERENCES	22

LIST OF TABLES

Table 1. Certified Values, Uncertainty & Tolerance Intervals for OREAS 920b.	2
Table 2. Indicative Values for OREAS 920b.	6
Table 3. Physical properties of OREAS 920b.	9
Table 4. Performance Gates for OREAS 920b.	11

LIST OF FIGURES

Figure 1. Cu by 4-acid digestion in OREAS 920b	16
--	----

INTRODUCTION

OREAS reference materials are intended to provide a low-cost method of evaluating and improving the quality of analysis of geological samples. To the geologist they provide a means of implementing quality control in analytical data sets generated in exploration from the grass roots level through to prospect evaluation, and in grade control at mining operations. To the analyst they provide an effective means of calibrating analytical equipment, assessing new techniques and routinely monitoring in-house procedures. OREAS reference materials enable users to successfully achieve process control of these tasks because the observed variance from repeated analysis has its origin almost exclusively in the analytical process rather than the reference material itself. In evaluating laboratory performance with this CRM, the section headed 'Instructions for correct use' should be read carefully.

Tables 1 provide the certified values and their associated 95% expanded uncertainty and tolerance intervals, Table 2 shows indicative values including major and trace element characterisation, Table 3 provides some indicative physical properties and Table 4 presents the performance gate intervals for all certified values.

Tabulated results of all analytes together with uncorrected means, medians, standard deviations, relative standard deviations and per cent deviation of lab means from the corrected mean of means (PDM³) are presented in the detailed certification data for this CRM (**OREAS 920b-DataPack.1.0.230602_164255.xlsx**).

Results are also presented in scatter plots for copper 4-acid digestion (Figure 1) together with $\pm 3SD$ (magenta) and $\pm 5\%$ (yellow) control lines and certified value (green line). Accepted individual results are coloured blue and individual and dataset outliers are identified in red and violet, respectively.

SOURCE MATERIAL

OREAS 920b was prepared from a blend of barren black slate and mine waste rock. The barren black slate was sourced from a quarry located in Victoria, Australia and the mine waste rock was sourced from the CSA mine located near the town of Cobar in central western New South Wales, Australia. The copper ore body of the CSA mine is hosted by the Early Devonian CSA Siltstone, a thinly bedded turbiditic sequence of carbonaceous siltstones and mudstones with minor coarser units. Iron-rich chlorite and silica are prominent alterations in the siltstone host.

COMMINUTION AND HOMOGENISATION PROCEDURES

The material constituting OREAS 920b was prepared in the following manner:

- Drying of black slate and waste rock to constant mass at 105°C;
- Crushing and milling of black slate and waste rock to >98% minus 75 microns;
- Blending the black slate and waste rock in appropriate proportions to achieve the target Cu grade;
- Homogenisation using OREAS' novel processing technologies;
- Packaging into 10g units in laminated foil pouches.

PHYSICAL PROPERTIES

OREAS 920b was tested at ORE Research & Exploration Pty Ltd's onsite facility for various physical properties. Table 3 presents these findings that should be used for informational purposes only.

Table 3. Physical properties of OREAS 920b.

Bulk Density (kg/m ³)	Moisture (wt.%)	Munsell Notation [‡]	Munsell Color [‡]
975	0.62	N6	Medium Light Gray

[‡]The Munsell Rock Color Chart helps geologists and archeologists communicate with colour more effectively by cross-referencing ISCC-NBS colour names with unique Munsell alpha-numeric colour notations for rock colour samples.

ANALYTICAL PROGRAM

Twenty-three commercial analytical laboratories participated in the program to certify the elements reported in Table 1. The following methods were employed:

- 4-acid (HF-HNO₃-HClO₄-HCl) digestion for full ICP-OES and ICP-MS elemental suites (up to 23 laboratories depending on the element);
- Aqua regia digestion for full ICP-OES and ICP-MS elemental suites (up to 23 laboratories depending on the element);
- Peroxide fusion for full ICP-OES and ICP-MS elemental suites with the exception of one laboratory that used borate fusion with ICP-OES (up to 21 laboratories depending on the element).

For the round robin program ten 350g test units were taken at predetermined intervals during the bagging stage, immediately following homogenisation and are considered representative of the entire prepared batch. The six samples received by each laboratory were obtained by taking two 20g scoop splits from each of three separate 350g test units. This format enabled nested ANOVA treatment of the results to evaluate homogeneity, i.e., to ascertain whether between-unit variance is greater than within-unit variance.

STATISTICAL ANALYSIS

Standard Deviation intervals (see Table 1) provide an indication of a level of performance that might reasonably be expected from a laboratory being monitored by this CRM in a QA/QC program. They take into account errors attributable to measurement uncertainty and CRM variability. For an effective CRM the contribution of the latter should be negligible in comparison to measurement errors. The Standard Deviation values include all sources of measurement uncertainty: between-lab variance, within-run variance (precision errors) and CRM variability.

In the application of SD's in monitoring performance it is important to note that not all laboratories function at the same level of proficiency and that different methods in use at a particular laboratory have differing levels of precision. Each laboratory has its own inherent SD (for a specific concentration level and analyte-method pair) based on the analytical process and this SD is not directly related to the round robin program (see Intended Use section for more detail).

The SD for each analyte's certified value is calculated from the same filtered data set used to determine the certified value, i.e., after removal of all individual, lab dataset (batch) and 3SD outliers (single iteration). These outliers can only be removed after the absolute homogeneity of the CRM has been independently established, i.e., the outliers must be confidently deemed to be analytical rather than arising from inhomogeneity of the CRM. ***The standard deviation is then calculated for each analyte from the pooled accepted analyses generated from the certification program.***

Certified Values, Standard Deviations, Confidence Limits and Tolerance Limits (Table 1) have been determined for each analyte following removal of individual, laboratory dataset (batch) and 3SD outliers (single iteration). For individual outliers within a laboratory batch the z-score test is used in combination with a second method that determines the per cent deviation of the individual value from the batch median. Outliers in general are selected on the basis of z-scores > 2.5 and with per cent deviations (i) > 3 and (ii) more than three times the average absolute per cent deviation for the batch. In certain instances, statistician's prerogative has been employed in discriminating outliers.

Each laboratory data set mean is tested for outlying status based on z-score discrimination and rejected if > 2.5. After individual and laboratory data set (batch) outliers have been eliminated a non-iterative 3 standard deviation filter is applied, with those values lying outside this window also relegated to outlying status.

95% Confidence Limits are inversely proportional to the number of participating laboratories and inter-laboratory agreement. It is a measure of the reliability of the certified value. A 95% confidence interval indicates a 95% probability that the true value of the analyte under consideration lies between the upper and lower limits. ***95% Confidence Limits should not be used as control limits for laboratory performance.***

Indicative (uncertified) values (Table 2) are present where the number of laboratories reporting a particular analyte is insufficient (< 5) to support certification or where inter-laboratory consensus is poor.

PERFORMANCE GATES

Table 4 below shows intervals calculated for two and three standard deviations. As a guide these intervals may be regarded as warning or rejection for multiple 2SD outliers, or rejection for individual 3SD outliers in QC monitoring, although their precise application should be at the discretion of the QC manager concerned (also see 'Intended Use' section below). Westgard Rules extend the basics of single-rule QC monitoring using multi-rules (for more information visit www.westgard.com/mltirule.htm). A second method utilises a 5% window calculated directly from the certified value.

Standard deviation is also shown in relative percent for one, two and three relative standard deviations (1RSD, 2RSD and 3RSD) to facilitate an appreciation of the magnitude of these numbers and a comparison with the 5% window. Caution should be exercised when concentration levels approach lower limits of detection of the analytical methods employed as performance gates calculated from standard deviations tend to be excessively wide whereas those determined by the 5% method are too narrow. One approach used at commercial laboratories is to set the acceptance criteria at twice the detection level (DL) \pm 10%.

i.e., Certified Value \pm 10% \pm 2DL [1].

Table 4. Performance Gates for OREAS 920b.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5% window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
4-Acid Digestion											
Ag, ppm	0.320	0.019	0.282	0.359	0.263	0.378	6.01%	12.02%	18.03%	0.304	0.336
Al, wt. %	6.79	0.251	6.29	7.29	6.04	7.54	3.69%	7.38%	11.07%	6.45	7.13
As, ppm	113	7	99	128	92	135	6.32%	12.65%	18.97%	108	119
Ba, ppm	2105	97	1912	2299	1815	2396	4.60%	9.19%	13.79%	2000	2211
Be, ppm	2.59	0.252	2.08	3.09	1.83	3.34	9.73%	19.47%	29.20%	2.46	2.72
Bi, ppm	0.79	0.048	0.70	0.89	0.65	0.94	6.08%	12.15%	18.23%	0.75	0.83
Ca, wt. %	0.030	0.000	0.030	0.030	0.030	0.030	0.00%	0.00%	0.00%	0.029	0.032
Cd, ppm	0.042	0.014	0.014	0.070	0.000	0.084	33.07%	66.15%	99.22%	0.040	0.044
Ce, ppm	90	3.4	83	97	80	100	3.73%	7.47%	11.20%	85	94
Co, ppm	1.63	0.088	1.45	1.80	1.37	1.89	5.38%	10.76%	16.14%	1.55	1.71
Cr, ppm	87	12	64	111	52	123	13.54%	27.07%	40.61%	83	92
Cs, ppm	4.43	0.246	3.93	4.92	3.69	5.16	5.56%	11.12%	16.68%	4.20	4.65
Cu, ppm	116	5	105	127	100	132	4.62%	9.23%	13.85%	110	122
Dy, ppm	3.62	0.53	2.56	4.68	2.03	5.21	14.62%	29.24%	43.86%	3.44	3.80
Er, ppm	1.72	0.095	1.53	1.92	1.44	2.01	5.52%	11.04%	16.56%	1.64	1.81
Eu, ppm	1.29	0.124	1.04	1.54	0.92	1.66	9.65%	19.29%	28.94%	1.22	1.35
Fe, wt. %	3.03	0.104	2.82	3.23	2.72	3.34	3.43%	6.87%	10.30%	2.88	3.18
Ga, ppm	20.3	1.02	18.3	22.4	17.3	23.4	5.01%	10.03%	15.04%	19.3	21.4
Gd, ppm	5.49	0.64	4.21	6.76	3.57	7.40	11.63%	23.25%	34.88%	5.21	5.76
Hf, ppm	2.32	0.148	2.03	2.62	1.88	2.77	6.37%	12.75%	19.12%	2.21	2.44
Ho, ppm	0.61	0.034	0.54	0.68	0.51	0.71	5.57%	11.14%	16.72%	0.58	0.64
In, ppm	0.075	0.009	0.057	0.094	0.048	0.103	12.11%	24.23%	36.34%	0.072	0.079
K, wt. %	2.71	0.081	2.55	2.87	2.47	2.95	2.98%	5.95%	8.93%	2.57	2.85
La, ppm	43.5	1.54	40.4	46.5	38.8	48.1	3.54%	7.08%	10.61%	41.3	45.6
Li, ppm	21.3	1.23	18.9	23.8	17.7	25.0	5.75%	11.51%	17.26%	20.3	22.4
Lu, ppm	0.26	0.020	0.22	0.31	0.20	0.33	7.57%	15.15%	22.72%	0.25	0.28
Mg, wt. %	0.377	0.020	0.337	0.416	0.317	0.436	5.23%	10.46%	15.69%	0.358	0.395
Mn, wt. %	0.007	0.000	0.007	0.008	0.006	0.008	4.37%	8.75%	13.12%	0.007	0.007
Mo, ppm	2.93	0.177	2.58	3.29	2.40	3.46	6.02%	12.05%	18.07%	2.79	3.08
Na, wt. %	0.098	0.014	0.070	0.125	0.056	0.139	14.17%	28.35%	42.52%	0.093	0.102
Nb, ppm	5.04	1.67	1.71	8.38	0.04	10.05	33.10%	66.20%	99.30%	4.79	5.30
Nd, ppm	36.2	3.16	29.8	42.5	26.7	45.6	8.74%	17.48%	26.21%	34.3	38.0
Ni, ppm	12.1	0.45	11.2	13.0	10.7	13.4	3.70%	7.41%	11.11%	11.5	12.7
P, wt. %	0.032	0.001	0.029	0.035	0.027	0.036	4.66%	9.32%	13.98%	0.030	0.034
Pb, ppm	26.4	1.55	23.3	29.5	21.7	31.1	5.89%	11.77%	17.66%	25.1	27.7
Pr, ppm	10.1	1.2	7.7	12.5	6.5	13.7	11.91%	23.81%	35.72%	9.6	10.6
Rb, ppm	156	8	139	172	131	181	5.31%	10.63%	15.94%	148	163
Re, ppm	< 0.002	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
S, wt. %	0.029	0.002	0.024	0.034	0.022	0.036	8.06%	16.11%	24.17%	0.028	0.031
Sb, ppm	3.97	0.278	3.42	4.53	3.14	4.81	7.00%	13.99%	20.99%	3.77	4.17
Sc, ppm	12.5	0.74	11.0	14.0	10.3	14.7	5.95%	11.91%	17.86%	11.9	13.1
Se, ppm	2.37	0.44	1.48	3.25	1.04	3.69	18.63%	37.25%	55.88%	2.25	2.48
Sm, ppm	7.09	0.644	5.81	8.38	5.16	9.03	9.08%	18.17%	27.25%	6.74	7.45

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg \equiv μ g/g \equiv 0.0001 wt. %.

Note 1: intervals may appear asymmetric due to rounding; IND = indeterminate.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Table 4 continued.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5% window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
4-Acid Digestion continued											
Sn, ppm	3.91	0.225	3.46	4.36	3.24	4.59	5.75%	11.50%	17.24%	3.72	4.11
Sr, ppm	57	2.9	51	63	48	66	5.14%	10.27%	15.41%	54	60
Ta, ppm	0.40	0.14	0.13	0.67	0.00	0.81	33.57%	67.14%	100.71%	0.38	0.42
Tb, ppm	0.71	0.09	0.53	0.88	0.45	0.97	12.22%	24.45%	36.67%	0.67	0.74
Te, ppm	0.088	0.017	0.054	0.123	0.037	0.140	19.55%	39.09%	58.64%	0.084	0.093
Th, ppm	15.5	1.25	13.0	18.0	11.7	19.2	8.04%	16.08%	24.13%	14.7	16.3
Ti, wt. %	0.226	0.035	0.156	0.296	0.121	0.331	15.43%	30.87%	46.30%	0.215	0.237
Tl, ppm	0.85	0.041	0.77	0.93	0.73	0.98	4.82%	9.64%	14.47%	0.81	0.89
Tm, ppm	0.25	0.04	0.18	0.32	0.15	0.36	14.13%	28.26%	42.39%	0.24	0.27
U, ppm	4.06	0.214	3.64	4.49	3.42	4.71	5.26%	10.52%	15.78%	3.86	4.27
V, ppm	166	9	149	184	140	192	5.26%	10.52%	15.78%	158	174
W, ppm	1.91	0.26	1.39	2.43	1.13	2.69	13.66%	27.33%	40.99%	1.81	2.00
Y, ppm	15.5	1.6	12.2	18.7	10.6	20.3	10.44%	20.89%	31.33%	14.7	16.2
Yb, ppm	1.61	0.152	1.31	1.92	1.16	2.07	9.38%	18.77%	28.15%	1.53	1.70
Zn, ppm	57	2.8	51	62	48	65	4.94%	9.87%	14.81%	54	60
Zr, ppm	80	4.5	71	89	66	93	5.66%	11.33%	16.99%	76	84
Aqua Regia Digestion											
Ag, ppm	0.174	0.012	0.150	0.198	0.138	0.210	6.87%	13.75%	20.62%	0.166	0.183
Al, wt. %	0.749	0.074	0.600	0.898	0.525	0.972	9.94%	19.88%	29.83%	0.711	0.786
As, ppm	111	6	99	123	93	129	5.38%	10.76%	16.14%	105	116
Au, ppm	0.019	0.005	0.009	0.029	0.004	0.034	25.78%	51.57%	77.35%	0.018	0.020
B, ppm	< 10	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Ba, ppm	190	34	122	258	88	292	17.91%	35.81%	53.72%	180	199
Be, ppm	0.52	0.08	0.37	0.67	0.29	0.75	14.60%	29.21%	43.81%	0.49	0.55
Bi, ppm	0.59	0.06	0.47	0.71	0.41	0.77	10.20%	20.39%	30.59%	0.56	0.62
Ca, wt. %	0.023	0.004	0.015	0.030	0.011	0.034	17.00%	34.00%	50.99%	0.022	0.024
Cd, ppm	0.033	0.008	0.017	0.049	0.009	0.057	23.95%	47.90%	71.85%	0.032	0.035
Ce, ppm	79	4.8	69	89	65	93	6.07%	12.13%	18.20%	75	83
Co, ppm	1.47	0.126	1.21	1.72	1.09	1.84	8.60%	17.20%	25.80%	1.39	1.54
Cr, ppm	23.1	1.25	20.6	25.6	19.3	26.8	5.41%	10.81%	16.22%	21.9	24.2
Cs, ppm	1.08	0.16	0.76	1.41	0.59	1.57	15.03%	30.05%	45.08%	1.03	1.14
Cu, ppm	115	6	104	126	98	132	4.88%	9.75%	14.63%	109	121
Fe, wt. %	2.77	0.155	2.45	3.08	2.30	3.23	5.61%	11.22%	16.82%	2.63	2.90
Ga, ppm	2.64	0.44	1.77	3.51	1.33	3.94	16.52%	33.05%	49.57%	2.51	2.77
Hf, ppm	0.35	0.05	0.25	0.45	0.20	0.50	14.12%	28.23%	42.35%	0.33	0.37
In, ppm	0.024	0.004	0.017	0.032	0.013	0.036	15.20%	30.39%	45.59%	0.023	0.026
K, wt. %	0.263	0.041	0.180	0.346	0.139	0.387	15.74%	31.47%	47.21%	0.250	0.276
La, ppm	33.0	2.33	28.3	37.7	26.0	40.0	7.07%	14.14%	21.21%	31.4	34.7
Li, ppm	2.90	0.41	2.08	3.72	1.67	4.14	14.17%	28.35%	42.52%	2.76	3.05
Lu, ppm	0.11	0.01	0.08	0.14	0.07	0.16	12.75%	25.51%	38.26%	0.11	0.12
Mg, wt. %	0.088	0.010	0.069	0.108	0.059	0.118	11.07%	22.14%	33.21%	0.084	0.093
Mn, wt. %	0.005	0.000	0.004	0.006	0.004	0.006	6.72%	13.43%	20.15%	0.005	0.005
Mo, ppm	2.75	0.169	2.41	3.08	2.24	3.25	6.13%	12.27%	18.40%	2.61	2.88

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt. % (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding; IND = indeterminate.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Table 4 continued.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5% window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
Aqua Regia Digestion continued											
Nb, ppm	0.054	0.007	0.040	0.067	0.033	0.074	12.70%	25.40%	38.09%	0.051	0.056
Ni, ppm	9.00	0.613	7.77	10.22	7.16	10.83	6.82%	13.63%	20.45%	8.55	9.44
P, wt. %	0.026	0.002	0.022	0.031	0.019	0.034	8.86%	17.72%	26.59%	0.025	0.028
Pb, ppm	16.6	1.46	13.7	19.5	12.3	21.0	8.76%	17.51%	26.27%	15.8	17.5
Rb, ppm	15.6	1.6	12.4	18.8	10.8	20.4	10.26%	20.53%	30.79%	14.8	16.4
Re, ppm	< 0.001	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
S, wt. %	0.026	0.005	0.016	0.035	0.012	0.040	18.36%	36.72%	55.08%	0.025	0.027
Sb, ppm	2.54	0.46	1.63	3.45	1.17	3.90	17.96%	35.92%	53.87%	2.41	2.66
Sc, ppm	1.57	0.21	1.14	2.00	0.93	2.21	13.64%	27.28%	40.92%	1.49	1.65
Se, ppm	2.24	0.199	1.84	2.64	1.65	2.84	8.86%	17.72%	26.58%	2.13	2.35
Sn, ppm	0.59	0.12	0.34	0.83	0.22	0.96	20.90%	41.81%	62.71%	0.56	0.62
Sr, ppm	14.0	2.8	8.4	19.6	5.6	22.4	19.92%	39.85%	59.77%	13.3	14.7
Ta, ppm	< 0.01	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Tb, ppm	0.50	0.027	0.45	0.55	0.42	0.58	5.32%	10.64%	15.97%	0.47	0.52
Te, ppm	0.071	0.012	0.048	0.095	0.037	0.106	16.26%	32.52%	48.78%	0.068	0.075
Th, ppm	10.4	0.76	8.9	12.0	8.2	12.7	7.29%	14.57%	21.86%	9.9	11.0
Ti, wt. %	0.011	0.002	0.006	0.015	0.003	0.018	22.66%	45.33%	67.99%	0.010	0.011
Tl, ppm	0.10	0.01	0.08	0.13	0.07	0.14	12.30%	24.60%	36.90%	0.10	0.11
U, ppm	2.39	0.152	2.08	2.69	1.93	2.84	6.38%	12.76%	19.14%	2.27	2.51
V, ppm	19.3	1.9	15.4	23.2	13.5	25.1	10.08%	20.15%	30.23%	18.3	20.3
W, ppm	0.11	0.02	0.06	0.15	0.04	0.18	21.52%	43.03%	64.55%	0.10	0.11
Y, ppm	7.25	0.585	6.08	8.42	5.50	9.01	8.07%	16.14%	24.22%	6.89	7.61
Zn, ppm	47.5	2.36	42.8	52.2	40.4	54.6	4.97%	9.93%	14.90%	45.2	49.9
Zr, ppm	12.2	1.6	8.9	15.4	7.3	17.0	13.37%	26.74%	40.11%	11.5	12.8
Borate / Peroxide Fusion ICP											
Ag, ppm	< 5	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Al, wt. %	6.98	0.140	6.70	7.26	6.56	7.40	2.01%	4.02%	6.03%	6.63	7.33
As, ppm	110	12	85	134	72	147	11.36%	22.72%	34.08%	104	115
B, ppm	138	9	121	156	112	164	6.34%	12.68%	19.03%	131	145
Ba, ppm	2114	76	1963	2266	1887	2342	3.59%	7.18%	10.77%	2009	2220
Be, ppm	2.48	0.46	1.56	3.40	1.10	3.87	18.61%	37.23%	55.84%	2.36	2.61
Bi, ppm	0.87	0.16	0.56	1.19	0.40	1.34	18.12%	36.24%	54.36%	0.83	0.91
Ca, wt. %	< 0.1	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Ce, ppm	92	5.2	81	102	76	107	5.67%	11.35%	17.02%	87	96
Co, ppm	1.76	0.26	1.24	2.27	0.98	2.53	14.73%	29.46%	44.18%	1.67	1.84
Cr, ppm	109	19	71	146	52	165	17.34%	34.69%	52.03%	103	114
Cs, ppm	4.52	0.289	3.94	5.10	3.65	5.39	6.39%	12.79%	19.18%	4.30	4.75
Cu, ppm	119	17	85	153	68	170	14.27%	28.55%	42.82%	113	125
Dy, ppm	4.96	0.439	4.08	5.84	3.64	6.27	8.85%	17.70%	26.55%	4.71	5.21
Er, ppm	2.79	0.201	2.39	3.20	2.19	3.40	7.21%	14.42%	21.63%	2.65	2.93
Eu, ppm	1.31	0.16	0.99	1.62	0.83	1.78	12.15%	24.29%	36.44%	1.24	1.37
Fe, wt. %	3.03	0.092	2.85	3.22	2.76	3.31	3.03%	6.05%	9.08%	2.88	3.18
Ga, ppm	20.5	1.34	17.8	23.2	16.5	24.5	6.55%	13.11%	19.66%	19.5	21.5

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt. % (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding; IND = indeterminate.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Table 4 continued.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5% window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
Borate / Peroxide Fusion ICP continued											
Gd, ppm	5.81	0.65	4.51	7.11	3.86	7.76	11.17%	22.34%	33.50%	5.52	6.10
Ge, ppm	2.33	0.32	1.68	2.97	1.36	3.29	13.87%	27.74%	41.60%	2.21	2.44
Ho, ppm	0.97	0.065	0.84	1.10	0.78	1.17	6.69%	13.37%	20.06%	0.92	1.02
In, ppm	< 0.2	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
K, wt. %	2.76	0.127	2.51	3.01	2.38	3.14	4.61%	9.21%	13.82%	2.62	2.90
La, ppm	43.6	3.53	36.5	50.7	33.0	54.2	8.10%	16.20%	24.30%	41.4	45.8
Li, ppm	21.7	2.14	17.5	26.0	15.3	28.1	9.84%	19.68%	29.52%	20.6	22.8
Lu, ppm	0.41	0.04	0.33	0.49	0.28	0.53	10.04%	20.07%	30.11%	0.39	0.43
Mg, wt. %	0.387	0.013	0.361	0.414	0.348	0.427	3.38%	6.76%	10.15%	0.368	0.407
Mn, wt. %	0.008	0.000	0.007	0.008	0.006	0.009	4.99%	9.98%	14.97%	0.007	0.008
Mo, ppm	3.37	0.76	1.86	4.89	1.10	5.64	22.48%	44.97%	67.45%	3.20	3.54
Nb, ppm	12.2	1.15	9.9	14.5	8.7	15.6	9.47%	18.93%	28.40%	11.5	12.8
Nd, ppm	36.7	3.20	30.3	43.1	27.1	46.3	8.73%	17.47%	26.20%	34.8	38.5
P, wt. %	0.032	0.005	0.022	0.041	0.018	0.046	14.91%	29.81%	44.72%	0.030	0.033
Pb, ppm	30.3	5.1	20.2	40.5	15.1	45.5	16.75%	33.50%	50.25%	28.8	31.8
Pr, ppm	9.90	0.602	8.69	11.10	8.09	11.70	6.08%	12.16%	18.24%	9.40	10.39
Rb, ppm	154	6	142	166	135	172	3.96%	7.93%	11.89%	146	161
Re, ppm	< 0.1	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
S, wt. %	0.035	0.012	0.010	0.059	0.000	0.072	36.04%	72.08%	108.12%	0.033	0.036
Sb, ppm	4.10	0.259	3.58	4.62	3.32	4.88	6.31%	12.63%	18.94%	3.90	4.31
Sc, ppm	12.0	1.01	9.9	14.0	8.9	15.0	8.42%	16.84%	25.26%	11.4	12.6
Si, wt. %	35.16	0.833	33.50	36.83	32.66	37.66	2.37%	4.74%	7.11%	33.40	36.92
Sm, ppm	6.75	0.451	5.85	7.65	5.40	8.10	6.68%	13.35%	20.03%	6.41	7.09
Sr, ppm	60	4.5	52	69	47	74	7.37%	14.75%	22.12%	57	63
Ta, ppm	0.85	0.22	0.41	1.29	0.19	1.51	25.75%	51.49%	77.24%	0.81	0.89
Tb, ppm	0.83	0.067	0.70	0.97	0.63	1.04	8.06%	16.11%	24.17%	0.79	0.88
Te, ppm	< 1	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Th, ppm	14.7	1.33	12.0	17.3	10.7	18.6	9.05%	18.09%	27.14%	13.9	15.4
Ti, wt. %	0.330	0.013	0.304	0.357	0.291	0.370	4.00%	8.00%	12.00%	0.314	0.347
Tl, ppm	0.88	0.084	0.71	1.05	0.63	1.13	9.51%	19.02%	28.53%	0.84	0.92
Tm, ppm	0.42	0.034	0.35	0.49	0.32	0.52	8.16%	16.31%	24.47%	0.40	0.44
U, ppm	4.43	0.422	3.58	5.27	3.16	5.69	9.53%	19.06%	28.59%	4.21	4.65
V, ppm	176	9	158	195	148	205	5.33%	10.66%	15.99%	168	185
W, ppm	3.01	0.85	1.32	4.70	0.48	5.55	28.07%	56.14%	84.22%	2.86	3.16
Y, ppm	27.5	1.12	25.2	29.7	24.1	30.8	4.09%	8.18%	12.27%	26.1	28.8
Yb, ppm	2.75	0.187	2.38	3.13	2.19	3.31	6.79%	13.58%	20.37%	2.62	2.89
Zn, ppm	61	8	46	76	38	84	12.55%	25.09%	37.64%	58	64

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt. % (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding; IND = indeterminate.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Homogeneity Evaluation

The tolerance limits (ISO 16269:2014) shown in Tables 4 were determined using an analysis of precision errors method and are considered a conservative estimate of true homogeneity. The meaning of tolerance limits may be illustrated for copper by 4-acid digestion, where 99% of the time ($1-\alpha=0.99$) at least 95% of subsamples ($\rho=0.95$) will have concentrations lying between 113 and 119 ppm. Put more precisely, this means that if the same number of subsamples were taken and analysed in the same manner repeatedly, 99% of the tolerance intervals so constructed would cover at least 95% of the total population, and 1% of the tolerance intervals would cover less than 95% of the total population (ISO Guide 35).

Please note that tolerance limits pertain to the homogeneity of the CRM only and should not be used as control limits for laboratory performance.

The homogeneity of OREAS 920b has also been evaluated in a **nested ANOVA** of the round robin program. Each of the twenty-three round robin laboratories received six samples per CRM and these samples were made up of paired samples from three different, non-adjacent sampling intervals selected from the pool of ten 350g test units. The purpose of the ANOVA evaluation is to test that no statistically significant difference exists in the variance between-units to that of the variance within-units. This allows an assessment of homogeneity across the entire prepared batch of OREAS 920b. The test was performed using the following parameters:

- Null Hypothesis, H_0 : Between-unit variance is no greater than within-unit variance (reject H_0 if p -value < 0.05);
- Alternative Hypothesis, H_1 : Between-unit variance is greater than within-unit variance.


The datasets were filtered for both individual and laboratory data set (batch) outliers prior to the calculation of p -values. This process derived no significant p -values across the entire extent of certified values. The null hypothesis is retained.

Only results for constituents present in concentrations well above the detection levels (i.e., $>20 \times$ Lower Limit of Detection) for the various methods undertaken were considered for the objective of evaluating homogeneity. It is important to note that ANOVA is not an absolute measure of homogeneity. Rather, it establishes whether or not the analytes are distributed in a similar manner throughout the packaging run of OREAS 920b and whether the variance between two subsamples from the same unit is statistically distinguishable from the variance of two subsamples taken from any two separate units. A reference material therefore can possess poor absolute homogeneity yet still pass a relative homogeneity (ANOVA) test if the within-unit heterogeneity is large and similar across all units.

Based on the statistical analysis of the results of the inter-laboratory certification program it can be concluded that OREAS 920b is fit-for-purpose as a certified reference material (see 'Intended Use' below).

Figure 1. Cu by 4-Acid Digestion in OREAS 920b

SPC.1652.Cobar Cu CRMs.OREAS 920b.1.4-Acid.Cu.Lab.230606.083817.SN

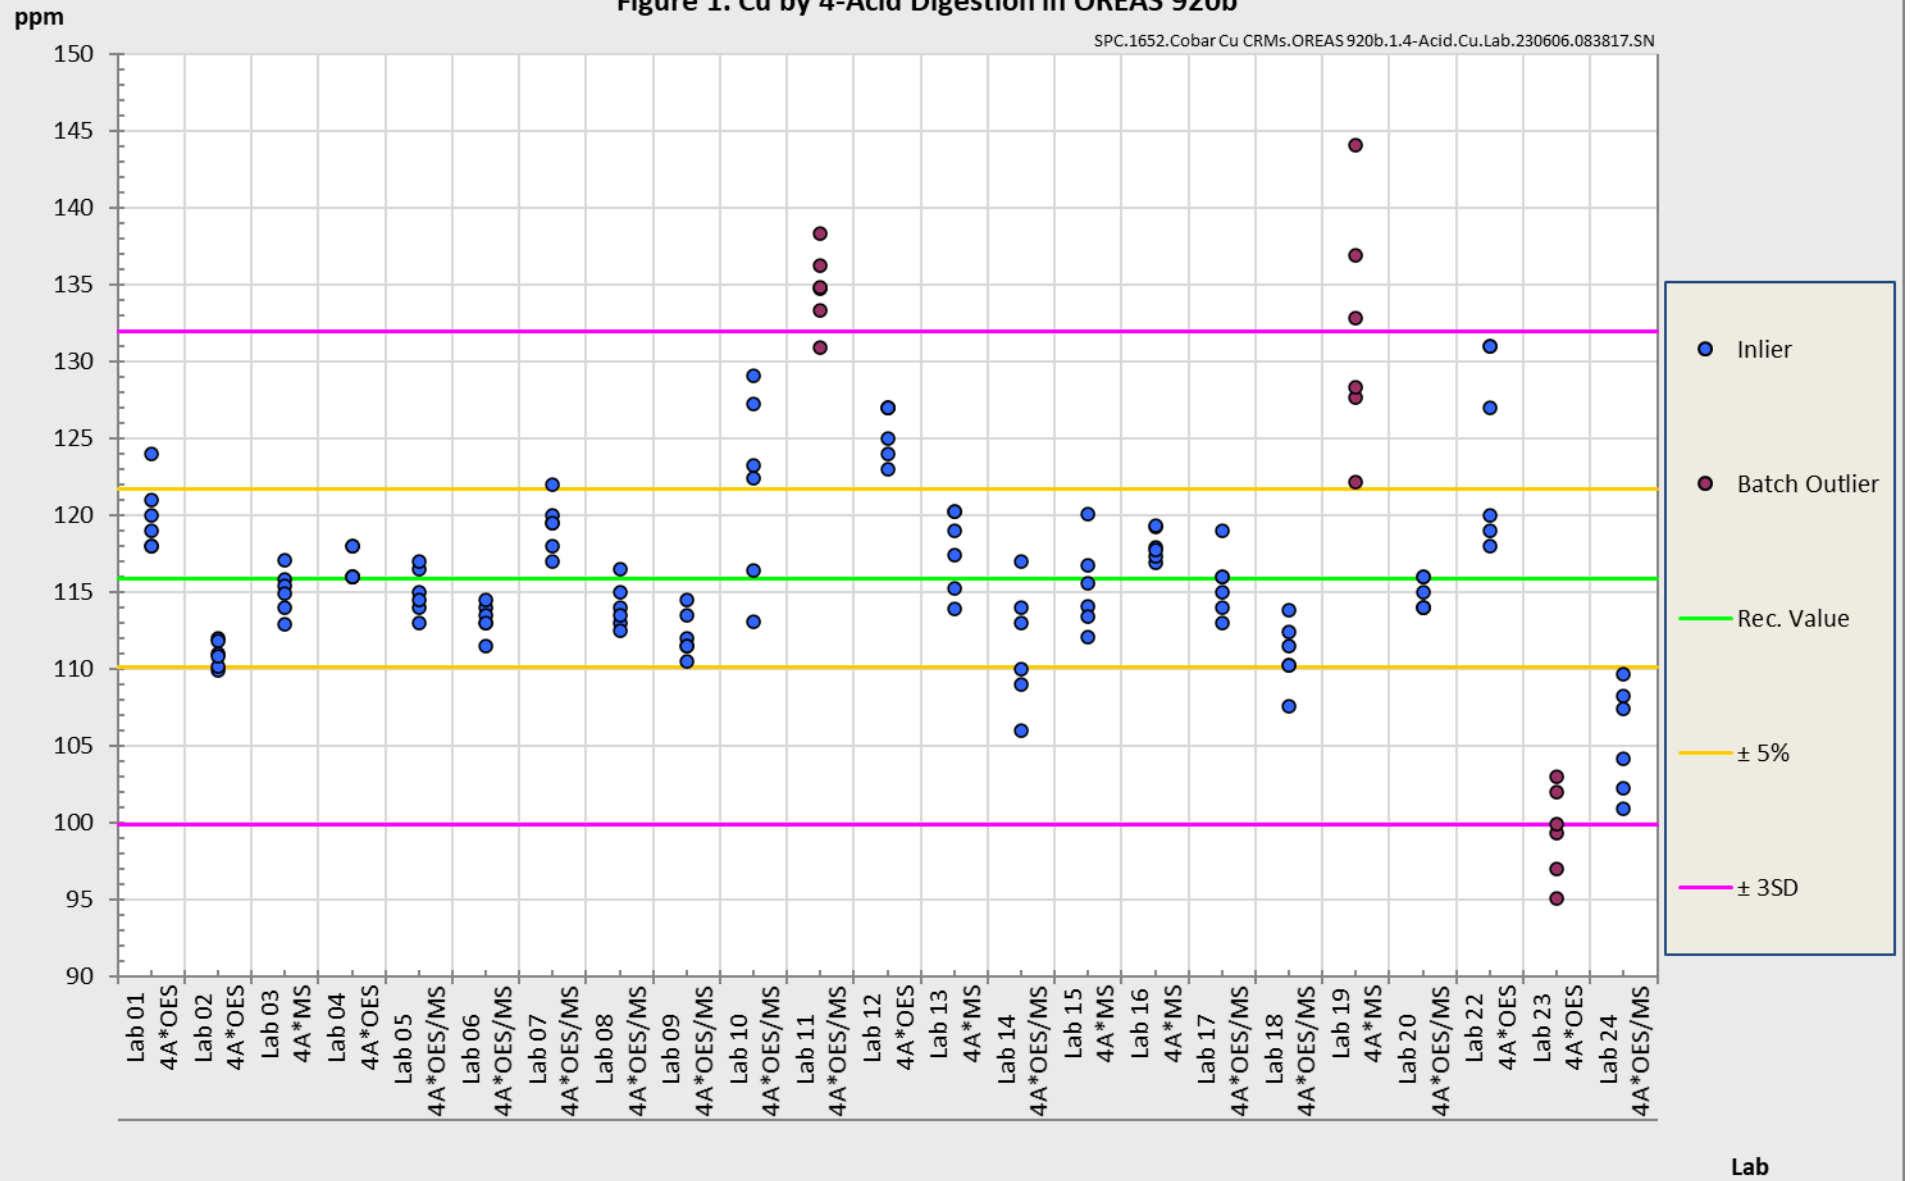

PARTICIPATING LABORATORIES

1. Actlabs, Ancaster, Ontario, Canada
2. AGAT Laboratories, Calgary, Alberta, Canada
3. ALS, Brisbane, QLD, Australia
4. ALS, Lima, Peru
5. ALS, Loughrea, Galway, Ireland
6. ALS, Perth, WA, Australia
7. ALS, Vancouver, BC, Canada
8. American Assay Laboratories, Sparks, Nevada, USA
9. Bureau Veritas Commodities Canada Ltd, Vancouver, BC, Canada
10. ESAN Istanbul, Istanbul, Turkey
11. Inspectorate (BV), Lima, Peru
12. Intertek Genalysis, Perth, WA, Australia
13. Intertek Testing Services, Townsville, QLD, Australia
14. Intertek Testing Services Philippines, Cupang, Muntinlupa, Philippines
15. MSALABS, Vancouver, BC, Canada
16. PT Geoservices Ltd, Cikarang, Jakarta Raya, Indonesia
17. PT Intertek Utama Services, Jakarta Timur, DKI Jakarta, Indonesia
18. Saskatchewan Research Council, Saskatoon, Saskatchewan, Canada
19. SGS, Randfontein, Gauteng, South Africa
20. SGS Canada Inc., Vancouver, BC, Canada
21. SGS de Mexico SA de CV, Cd. Industrial, Durango, Mexico
22. SGS Geosol Laboratorios Ltda, Vespasiano, Minas Gerais, Brazil
23. UIS Analytical Services, Centurion, South Africa

Please note: To preserve anonymity, the above numbered alphabetical list of participating laboratories does not correspond with the Lab ID numbering on the scatter plots below.

PREPARER AND SUPPLIER

Certified reference material OREAS 920b is prepared, certified and supplied by:



ORE Research & Exploration Pty Ltd
37A Hosie Street
Bayswater North VIC 3153
AUSTRALIA

Tel: +613-9729 0333
Fax: +613-9729 8338
Web: www.oreas.com
Email: info@ore.com.au

METROLOGICAL TRACEABILITY

The interlaboratory results that underpin the certified values are metrologically traceable to the international measurement scale (SI) of mass (either as a % mass fraction or as milligrams per kilogram (mg/kg)). In line with popular use, all data within tables in this

certificate are expressed as the mass fraction in either weight percent (wt.%) or parts per million (ppm).

The analytical samples sent to participating laboratories were selected in a manner to be representative of the entire prepared batch of CRM. This 'representivity' was maintained in each submitted laboratory sample batch and ensures the user that the data is traceable from sample selection through to the analytical results. The systematic sampling method was chosen due to the low risk of overlooking repetitive effects or trends in the batch due to the way the CRM was processed. In line with ISO 17025 [9], each analytical data set received from the participating laboratories has been validated by its assayer through the inclusion of internal reference materials and QC checks during and post analysis.

The participating laboratories were chosen on the basis of their competence (from past performance in interlaboratory programs undertaken by ORE Pty Ltd) for a particular analytical method, analyte or analyte suite and sample matrix. The operationally defined measurands characterised in this certificate are derived from data procured mostly from ISO 17025 accredited laboratories. The certified values presented in this report are calculated from the means of accepted data following robust technical and statistical analysis as detailed in this report.

Guide ISO/TR 16476:2016, section 5.3.1 describes metrological traceability in reference materials as it pertains to the transformation of the measurand. In this section it states, *"Although the determination of the property value itself can be made traceable to appropriate units through, for example, calibration of the measurement equipment used, steps like the transformation of the sample from one physical (chemical) state to another cannot. Such transformations may only be compared with a reference (when available), or among themselves. For some transformations, reference methods have been defined and may be used in certification projects to evaluate the uncertainty associated with such a transformation. In other cases, only a comparison among different laboratories using the same procedure is possible. In this case, it is impossible to demonstrate absence of method bias; therefore, the result is an operationally defined measurand (ISO Guide 35:2017, 9.2.4c)."* Certification takes place on the basis of agreement among operationally defined, independent measurement results.

COMMUTABILITY

The measurements of the results that underlie the certified values contained in this report were undertaken by methods involving pre-treatment (fusion/digestion) of the sample. This served to reduce the sample to a simple and well understood form permitting calibration using simple solutions of the CRM. Due to these methods being well understood and highly effective, commutability is not an issue for this CRM. All OREAS CRMs are sourced from natural ore minerals meaning they will display similar behaviour as routine 'field' samples in the relevant measurement process. Care should be taken to ensure 'matrix matching' as close as practically achievable. The matrix and mineralisation style of the CRM is described in the 'Source Material' section and users should select appropriate CRMs matching these attributes to the field samples being analysed.

INTENDED USE

OREAS 920b is intended to cover all activities needed to produce a measurement result. This includes extraction, possible separation steps and the actual measurement process (the signal producing step). OREAS 920b may be used to calibrate the entire procedure by producing a pure substance CRM transformed into a calibration solution. OREAS 920b is intended for the following uses:

- For the monitoring of laboratory performance in the analysis of analytes reported in Tables 1 and 2 in geological samples;
- For the verification of analytical methods for analytes reported in Tables 1 and 2;
- For the calibration of instruments used in the determination of the concentration of analytes reported in Tables 1 and 2. When a value provided in this certificate is used to calibrate a measurement process, the uncertainty associated with that value should be appropriately propagated into the user's uncertainty calculation. Users can determine an approximation of the standard uncertainty by calculating one fourth of the width of the Expanded Uncertainty interval given in this certificate (Expanded Uncertainty intervals are provided in Tables 1 and 2).

PERIOD OF VALIDITY & STORAGE INSTRUCTIONS

The certification of OREAS 920b remains valid, within the specified measurement uncertainties, until March 2033, provided the CRM is handled and stored in accordance with the instructions given below. This certification is nullified if the CRM is any way changed or contaminated.

Store in a clean and cool dry place away from direct sunlight.

Long-term stability will be monitored at appropriate intervals and purchasers notified if any changes are observed. The period of validity may well be indefinite and will be reassessed prior to expiry with the aim of extending the validity if possible.

Single-use sachets

Following analysis, it is the manufacturer's expectation that any remaining material is discarded unless the sachet is promptly resealed. It is the user's responsibility to prevent contamination and minimise exposure to the atmosphere.

Repeat-use packaging (e.g., 500g plastic jars)

After taking a subsample, users should replace the lid of the jar promptly and securely to prevent accidental spills and airborne contamination. OREAS 920b contains a non-hygroscopic* matrix with an indicative value for moisture provided to enable users to check for changes to stored material by determining moisture in the user's laboratory and comparing the result to the value in Table 3 in this certificate.

The stability of the CRM in regard to oxidation from the breakdown of sulphide minerals to sulphates is negligible given its low sulphur concentration (0.03 wt.% S).

*A non-hygroscopic matrix means exposure to atmospheres significantly different, in terms of temperature and humidity, from the climate during manufacturing should have negligible impact on the precision of results. Hygroscopic moisture is the amount of adsorbed moisture (weakly held H₂O- molecules on the surface of exposed material) following exposure to the local atmosphere. Usually, equilibration of material to the local atmosphere will only occur if the material is spread into a thin (~2mm thick) layer and left exposed for a period of 2 hours.

INSTRUCTIONS FOR HANDLING & CORRECT USE

Pre-homogenisation of the CRM prior to subsampling and analysis is not necessary as there is no particle segregation under transport [13]. Fine powders pose a risk to eyes and lungs and therefore standard precautions including the use of safety glasses and dust masks are advised. The certified values contained in this report refer to the concentration levels in the packaged state. There is no need for drying prior to weighing and analysis.

Minimum sample size

As a practical guide, the minimum mass of sample used should match the typical mass that the laboratories used in the interlaboratory (round robin) certification program. This means that different sample masses should be used depending on the operationally defined methodology.

- 4-acid digestion with ICP-OES and/or MS finish: $\geq 0.25\text{g}$;
- Aqua regia digestion with ICP-OES and/or MS finish: $\geq 0.5\text{g}$;
- Peroxide fusion for full elemental suite with ICP-OES and/or MS finish: $\geq 0.1\text{g}$.

QC monitoring using multiples of the Standard Deviation (SD)

In the application of SD's in monitoring performance it is important to note that not all laboratories function at the same level of proficiency and that different methods in use at a particular laboratory have differing levels of precision. Each laboratory has its own inherent SD (for a specific concentration level and analyte-method pair) based on the analytical process and this SD is not directly related to the round robin program.

The majority of data generated in the round robin program was produced by a selection of world class laboratories. The SD's thus generated are more constrained than those that would be produced across a randomly selected group of laboratories. To produce more generally achievable SD's the 'pooled' SD's provided in this report include inter-laboratory bias. This 'one size fits all' approach may require revision at the discretion of the QC manager concerned following careful scrutiny of QC control charts.

The performance gates shown in Table 4 are intended only to be used as an initial guide as to what a laboratory may be able to achieve. Over a period of time monitoring your own laboratory's data for this CRM, SDs should be calculated directly from your own laboratory's process. This will enable you to establish more specific performance gates that are fit for purpose for your application as well as the ability to monitor bias. If your long-term trend analysis shows an average value that is within the 95% confidence interval then generally there is no cause for concern in regard to bias.

For use with the aqua regia digestion method

It is important to note that in the analytical industry there is no standardisation of the aqua regia digestion process. This method is a partial empirical digest and differences in recoveries for various analytes are commonplace. These are caused by variations in the digest conditions and can include the ratio of nitric to hydrochloric acids, acid strength, temperatures, leach times and secondary digestions. Recoveries for sulphide-hosted base metal sulphides approach total values, however, other analytes, in particular the lithophile elements, show greater sensitivity to method parameters. This can result in lack of consensus in an inter-laboratory certification program for these elements.

The approach applied here is to report certified values in those instances where reasonable agreement exists amongst a majority of participating laboratories. The results of specific laboratories may differ significantly from the certified values, but will, nonetheless, be valid and reproducible in the context of the specifics of the aqua regia method in use. Users of this reference material should, therefore, be mindful of this limitation when applying the certified values in a quality control program.

LEGAL NOTICE

Ore Research & Exploration Pty Ltd has prepared and statistically evaluated the property values of this reference material to the best of its ability. The Purchaser by receipt hereof releases and indemnifies Ore Research & Exploration Pty Ltd from and against all liability and costs arising from the use of this material and information.

© COPYRIGHT Ore Research & Exploration Pty Ltd. Unauthorised copying, reproduction, storage or dissemination is prohibited.

DOCUMENT HISTORY


Revision No.	Date	Changes applied
1	2 nd August, 2023	Changed the description on the title page from 'Copper ore' to 'Copper-bearing siltstone'.
0	28 th June, 2023	First publication.

QMS CERTIFICATION

ORE Pty Ltd is accredited for compliance with ISO 17034.



ORE Pty Ltd is ISO 9001:2015 certified by Lloyd's Register Quality Assurance Ltd for its quality management system including development, manufacturing, certification and supply of CRMs.

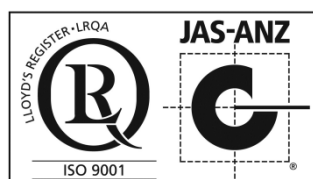

CERTIFYING OFFICER



28th June, 2023

Craig Hamlyn (B.Sc. Hons - Geology), Technical Manager - ORE P/L

REFERENCES

- [1] Govett, G.J.S. (1983). Handbook of Exploration Geochemistry, Volume 2: Statistics and Data Analysis in Geochemical Prospecting (Variations of accuracy and precision).
- [2] Ingamells, C. O. and Switzer, P. (1973). A Proposed Sampling Constant for Use in Geochemical Analysis, Talanta 20, 547-568.
- [3] ISO Guide 30:2015. Terms and definitions used in connection with reference materials.
- [4] ISO Guide 31:2015. Reference materials – Contents of certificates and labels.
- [5] ISO Guide 35:2017. Certification of reference materials - General and statistical principals.
- [6] ISO Guide 98-3:2008. Guide to the expression of uncertainty in measurement (GUM:1995).
- [7] ISO 16269-6:2014, Statistical interpretation of data – Determination of statistical tolerance intervals.
- [8] ISO/TR 16476:2016, Reference Materials – Establishing and expressing metrological traceability of quantity values assigned to reference materials.
- [9] ISO 17025:2017, General requirements for the competence of testing and calibration laboratories.
- [10] ISO Guide 17034:2016. General requirements for the competence of reference material producers.
- [11] Munsell Rock Color Book (2014). Rock-Color Chart Committee, Geological Society of America (GSA), Minnesota (USA).
- [12] OREAS-BUP-70-09-11: Statistical Analysis - OREAS Evaluation Method.
- [13] OREAS-TN-04-1498: Stability under transport; an experimental study of OREAS CRMs.
- [14] OREAS-TN-05-1674: Long-term storage stability; an experimental study of OREAS CRMs.
- [15] Thompson, A.; Taylor, B.N.; Guide for the Use of the International System of Units (SI); NIST Special Publication 811; U.S. Government Printing Office: Washington, DC (2008); available at: <https://physics.nist.gov/cuu/pdf/sp811.pdf> (accessed Nov 2021).
- [16] Van der Veen AMH and Pauwels, J. (2001), Accred Qual Assur 6: 290-294.