

CERTIFICATE OF ANALYSIS FOR

CERTIFIED REFERENCE MATERIAL


OREAS 181b

Lateritic Nickel-Cobalt Ore

(Northeastern Goldfields of Western Australia)



Accredited for compliance with ISO 17034



COA-1805-OREAS 181b-R1
BUP-70-10-01 Ver:2.0

14-Aug-2025

Table 1. Certified Values, Uncertainty & Tolerance Intervals for OREAS 181b.

Constituent	Certified Value†	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
Borate Fusion XRF					
Al2O3, Aluminium(III) oxide (wt.%)	7.20	7.11	7.28	7.14	7.25
BaO, Barium oxide (ppm)	238	167	310	IND	IND
CaO, Calcium oxide (wt.%)	0.364	0.355	0.373	0.357	0.371
Co, Cobalt (ppm)	458	443	473	444	472
Cr2O3, Chromium(III) oxide (wt.%)	0.657	0.645	0.669	0.649	0.665
Cu, Copper (ppm)	< 50	IND	IND	IND	IND
Fe2O3, Iron(III) oxide (wt.%)	34.61	34.31	34.91	34.41	34.81
K2O, Potassium oxide (wt.%)	0.733	0.719	0.747	0.720	0.746
MgO, Magnesium oxide (wt.%)	5.77	5.72	5.82	5.74	5.81
MnO, Manganese oxide (wt.%)	0.174	0.171	0.178	0.172	0.177
Na2O, Sodium oxide (wt.%)	0.330	0.306	0.353	0.318	0.341
Ni, Nickel (wt.%)	0.520	0.508	0.532	0.514	0.526
P2O5, Phosphorus(V) oxide (wt.%)	0.035	0.031	0.040	0.033	0.038
SiO2, Silicon dioxide (wt.%)	38.83	38.45	39.21	38.63	39.03
Sn, Tin (ppm)	< 50	IND	IND	IND	IND
SO3, Sulphur trioxide (wt.%)	0.267	0.247	0.288	0.257	0.278
TiO2, Titanium dioxide (wt.%)	0.332	0.323	0.342	0.324	0.341
V2O5, Vanadium(V) oxide (ppm)	165	111	220	IND	IND
Zn, Zinc (ppm)	92	72	112	IND	IND
Thermogravimetry					
LOI ¹⁰⁰⁰ , Loss on ignition @1000 °C (wt.%)	9.78	9.59	9.97	9.68	9.87
Borate / Peroxide Fusion ICP					
Al, Aluminium (wt.%)	3.74	3.67	3.81	3.69	3.79
As, Arsenic (ppm)	115	94	136	107	123
B, Boron (ppm)	354	304	405	341	368
Ba, Barium (ppm)	210	203	218	204	216
Be, Beryllium (ppm)	1.07	0.91	1.23	IND	IND
Bi, Bismuth (ppm)	4.89	3.64	6.14	4.16	5.62
Ca, Calcium (wt.%)	0.258	0.229	0.286	0.241	0.274
Cd, Cadmium (ppm)	< 10	IND	IND	IND	IND
Ce, Cerium (ppm)	34.1	29.4	38.7	32.3	35.8
Co, Cobalt (ppm)	442	420	464	434	450
Cr, Chromium (wt.%)	0.445	0.432	0.458	0.438	0.452
Cs, Caesium (ppm)	2.68	2.38	2.97	2.42	2.94
Cu, Copper (ppm)	40.7	37.3	44.2	36.8	44.7

SI unit equivalents: ppm (parts per million; 1×10^{-6}) $\equiv$ mg/kg; wt.% (weight per cent) $\equiv$ % (mass fraction).

Note: intervals may appear asymmetric due to rounding.

[†]These operationally defined measurands meet the requirements of ISO 17034 and all participating laboratories comply with the requirements of ISO 17025.

IND = indeterminate (due to limited reading resolution of the methods employed. For practical purposes the 95% Expanded Uncertainty can be set between zero and a two times multiple of the upper bound/non-detect limit value).

Table 1 continued.

Constituent	Certified Value†	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
Borate / Peroxide Fusion ICP continued					
Dy, Dysprosium (ppm)	2.08	1.86	2.30	1.94	2.22
Er, Erbium (ppm)	1.16	1.01	1.32	1.07	1.26
Eu, Europium (ppm)	0.54	0.42	0.66	0.49	0.59
Fe, Iron (wt.%)	24.12	23.45	24.78	23.77	24.46
Ga, Gallium (ppm)	9.38	8.31	10.46	8.94	9.83
Gd, Gadolinium (ppm)	2.07	1.78	2.37	1.89	2.26
Ge, Germanium (ppm)	1.78	1.01	2.55	IND	IND
Ho, Holmium (ppm)	0.40	0.36	0.43	0.37	0.43
In, Indium (ppm)	< 0.1	IND	IND	IND	IND
K, Potassium (wt.%)	0.626	0.575	0.678	0.604	0.648
La, Lanthanum (ppm)	13.7	12.1	15.4	12.8	14.7
Li, Lithium (ppm)	12.7	8.8	16.6	10.3	15.1
Lu, Lutetium (ppm)	0.16	0.11	0.20	IND	IND
Mg, Magnesium (wt.%)	3.40	3.30	3.49	3.35	3.44
Mn, Manganese (wt.%)	0.134	0.128	0.140	0.132	0.137
Mo, Molybdenum (ppm)	2.37	1.61	3.14	IND	IND
Nd, Neodymium (ppm)	11.2	10.4	11.9	10.6	11.8
Ni, Nickel (wt.%)	0.513	0.499	0.527	0.505	0.520
Pr, Praseodymium (ppm)	3.17	2.76	3.59	2.99	3.36
Rb, Rubidium (ppm)	33.4	31.4	35.4	32.0	34.8
Re, Rhenium (ppm)	< 0.1	IND	IND	IND	IND
S, Sulphur (wt.%)	0.097	0.074	0.121	0.088	0.107
Sc, Scandium (ppm)	19.8	18.7	20.8	18.6	20.9
Se, Selenium (ppm)	< 20	IND	IND	IND	IND
Si, Silicon (wt.%)	18.04	17.58	18.50	17.65	18.43
Sm, Samarium (ppm)	2.28	1.91	2.65	2.06	2.50
Sr, Strontium (ppm)	32.5	29.1	35.9	30.2	34.8
Tb, Terbium (ppm)	0.33	0.26	0.39	0.30	0.36
Te, Tellurium (ppm)	< 1	IND	IND	IND	IND
Th, Thorium (ppm)	4.62	4.02	5.23	4.42	4.83
Ti, Titanium (wt.%)	0.196	0.187	0.205	0.189	0.202
Tl, Thallium (ppm)	< 0.5	IND	IND	IND	IND
Tm, Thulium (ppm)	0.17	0.14	0.20	0.13	0.21
U, Uranium (ppm)	1.02	0.80	1.25	IND	IND
V, Vanadium (ppm)	85	78	91	81	88

SI unit equivalents: ppm (parts per million; 1×10^{-6}) $\equiv$ mg/kg; wt.% (weight per cent) $\equiv$ % (mass fraction).

Note: intervals may appear asymmetric due to rounding.

[†]These operationally defined measurands meet the requirements of ISO 17034 and all participating laboratories comply with the requirements of ISO 17025.

IND = indeterminate (due to limited reading resolution of the methods employed. For practical purposes the 95% Expanded Uncertainty can be set between zero and a two times multiple of the upper bound/non-detect limit value).

Table 1 continued.

Constituent	Certified Value†	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
Borate / Peroxide Fusion ICP continued					
W, Tungsten (ppm)	22.9	18.5	27.4	21.0	24.9
Y, Yttrium (ppm)	10.5	9.5	11.4	9.9	11.0
Yb, Ytterbium (ppm)	1.15	0.99	1.31	IND	IND
Zn, Zinc (ppm)	95	87	104	89	102
Infrared Combustion					
C, Carbon (wt.%)	1.10	1.07	1.12	1.08	1.11
S, Sulphur (wt.%)	0.102	0.092	0.112	0.099	0.105

SI unit equivalents: ppm (parts per million; 1×10^{-6}) $\equiv$ mg/kg; wt.% (weight per cent) $\equiv$ % (mass fraction).

Note: intervals may appear asymmetric due to rounding. IND = indeterminate.

[†]These operationally defined measurands meet the requirements of ISO 17034 and all participating laboratories comply with the requirements of ISO 17025.

Table 2. Indicative Values for OREAS 181b.

Constituent	Unit	Value	Constituent	Unit	Value	Constituent	Unit	Value
Borate Fusion XRF								
As	ppm	115	Hg	ppm	< 100	Se	ppm	< 100
Bi	ppm	< 100	In	ppm	< 100	SrO	ppm	< 120
Cd	ppm	< 100	La	ppm	< 90	Ta	ppm	< 100
Ce	ppm	81	Mo	ppm	< 50	Te	ppm	< 100
Cl	ppm	516	Nb	ppm	< 50	Tl	ppm	< 100
Cs	ppm	< 100	Pb	ppm	180	W	ppm	14.7
Ga	ppm	< 100	Rb	ppm	< 50	Y	ppm	< 39
Ge	ppm	< 100	Sb	ppm	< 50	Zr	ppm	82
HfO ₂	ppm	< 100	Sc	ppm	17.2			
Thermogravimetry								
H ₂ O-	wt.%	2.39						
Borate / Peroxide Fusion ICP								
Ag	ppm	< 0.5	Nb	ppm	4.38	Sn	ppm	4.07
Hf	ppm	2.46	P	wt.%	0.017	Ta	ppm	0.56
Hg	ppm	0.30	Pb	ppm	20.8	Zr	ppm	74
Na	wt.%	0.304	Sb	ppm	3.46			
4-Acid Digestion								
Co	ppm	460	Mg	wt.%	3.41			
Fe	wt.%	22.62	Ni	wt.%	0.525			

SI unit equivalents: ppm (parts per million; 1×10^{-6}) $\equiv$ mg/kg; wt.% (weight per cent) $\equiv$ % (mass fraction).

Note: the number of significant figures reported is not a reflection of the level of certainty of stated values. They are instead an artefact of ORE's in-house CRM-specific LIMS.

TABLE OF CONTENTS

INTRODUCTION	6
SOURCE MATERIAL.....	6
COMMINUTION AND HOMOGENISATION PROCEDURES	6
PHYSICAL PROPERTIES	7
MINERALOGY	7
ANALYTICAL PROGRAM.....	8
STATISTICAL ANALYSIS	8
Certified Values and their uncertainty intervals	8
Indicative (uncertified) values.....	8
Homogeneity Evaluation	9
PERFORMANCE GATES	10
PARTICIPATING LABORATORIES.....	12
PREPARER AND SUPPLIER.....	15
METROLOGICAL TRACEABILITY	15
COMMUTABILITY	16
INTENDED USE	16
MINIMUM SAMPLE SIZE	16
PERIOD OF VALIDITY & STORAGE INSTRUCTIONS.....	16
INSTRUCTIONS FOR HANDLING & CORRECT USE.....	17
LEGAL NOTICE	18
DOCUMENT HISTORY	19
CERTIFYING OFFICER.....	18
QMS CERTIFICATION	18
REFERENCES	18

LIST OF TABLES

Table 1. Certified Values, Uncertainty & Tolerance Intervals for OREAS 181b.	2
Table 2. Indicative Values for OREAS 181b.	4
Table 3. Physical properties of OREAS 181b.	7
Table 4. Indicative mineralogy of OREAS 181b by semi-quantitative XRD analysis.....	7
Table 5. Performance Gates for OREAS 181b.	10

LIST OF FIGURES

Figure 1. Ni by borate fusion XRF in OREAS 181b	13
Figure 2. Co by borate fusion XRF in OREAS 181b	14

INTRODUCTION

OREAS reference materials are intended to provide a low-cost method of evaluating and improving the quality of analysis of geological samples. To the geologist they provide a means of implementing quality control in analytical data sets generated in exploration from the grass roots level through to prospect evaluation, and in grade control at mining operations. To the analyst they provide an effective means of calibrating analytical equipment, assessing new techniques and routinely monitoring in-house procedures. OREAS reference materials enable users to successfully achieve process control of these tasks because the observed variance from repeated analysis has its origin almost exclusively in the analytical process rather than the reference material itself. In evaluating laboratory performance with this CRM, the section headed 'Instructions for correct use' should be read carefully.

Table 1 (generated from data supplied by ISO 17025 accredited laboratories for the analytical methods employed) provides the certified values and their associated 95 % expanded uncertainty and tolerance intervals, Table 2 shows indicative values, Table 3 provides some indicative physical properties, Table 4 shows indicative mineralogy by semi-quantitative XRD analysis and Table 5 presents performance gate intervals for all certified values.

Tabulated results of all analytes together with uncorrected means, medians, standard deviations, relative standard deviations and per cent deviation of lab means from the corrected mean of means (PDM³) are presented in the detailed certification data for this CRM (**OREAS 181b-DataPack.1.1.250814_101040.xlsx**). Results are also presented in scatter plots for Ni and Co by borate fusion XRF in Figures 1 and 2 respectively, together with ± 3 SD (magenta) and ± 5 % (yellow) control lines and certified value (green line). Accepted individual results are coloured blue and individual and dataset outliers are identified in red and violet, respectively.

SOURCE MATERIAL

OREAS 181b has been prepared from a blend of Ni-Co lateritic ores and barren siliclastic sedimentary rock sourced from Victoria, Australia. The Ni-Co lateritic ores were sourced predominantly from the north-eastern Goldfields of Western Australia. Minor additions of Ni-Co lateritic ores from other regions were also added. The lateritic ores formed from prolonged lateritic weathering of Archaean (Yilgarn Craton) olivine rich ultramafic/komatiite flows. Grades of >1% Ni were generated in zones of more intense weathering associated with faulting and bedrock alteration. Ni-Co nontronitic (Fe-Ni smectite clays) siliceous ores formed with a goethitic overprint in the upper laterite profile.

COMMINUTION AND HOMOGENISATION PROCEDURES

The material constituting OREAS 181b was prepared in the following manner:

- Drying to constant mass at 105 °C;
- Crushing and milling of the ore materials to 100 % minus 30 microns;
- Crushing and multi-stage milling of the barren rocks to >98% minus 75 microns;
- Blending the ores and barren materials in appropriate proportions to achieve desired grades;
- Homogenisation using OREAS' novel processing technologies;

- Packaging in 10 g units in laminated foil pouches and 500 g units in plastic wide-mouth jars.

PHYSICAL PROPERTIES

OREAS 181b was tested at ORE Research & Exploration Pty Ltd's onsite facility for various physical properties. Table 3 presents these findings that should be used for informational purposes only.

Table 3. Physical properties of OREAS 181b.

Bulk Density (kg/m ³)	Moisture (wt.%)	Munsell Notation [‡]	Munsell Color [‡]
689	2.56	5YR 5/6	Light Brown

[‡]The Munsell Rock Color Chart helps geologists and archeologists communicate with colour more effectively by cross-referencing ISCC-NBS colour names with unique Munsell alpha-numeric colour notations for rock colour samples.

MINERALOGY

The semi-quantitative XRD results shown in Table 4 below were undertaken by ALS Metallurgy in Balcatta, Western Australia. The results have been normalised to 100 % and represent the relative proportion of crystalline material. Totals greater or less than 100 % are due to rounding errors. A presence of some amorphous material is very likely. Clay mineral appears to be mainly smectite and vermiculite. Kandite group appears to be mainly kaolinite. A trace of dolomite - ankerite might be present. Fe-spinel appears to include a variety of Fe-bearing spinel group minerals, such as magnetite, magnesioferrite, chromite, trevorite, ulvospinel, titanomagnetite etc. Some maghemite and Ni-spinel (e.g. nichromite) may be present and are reported under Fe-spinel.

Table 4. Indicative mineralogy of OREAS 181b by semi-quantitative XRD analysis.

Mineral / Mineral Group	% (mass ratio)
Clay mineral	1
Chlorite	< 1
Kandite group	5
Serpentine	2
Annite - biotite - phlogopite	1
Muscovite	11
Clinopyroxene	< 1
Orthopyroxene	3
Plagioclase	1
K-feldspar and/or rutile	< 1
Tourmaline	1
Olivine	2
Quartz	28
Magnesite	12
Hematite	10
Goethite	17
Fe-spinel	5

ANALYTICAL PROGRAM

Twenty-six commercial analytical laboratories participated in the program to certify the elements reported in Table 1. The following methods were employed:

- Lithium borate fusion whole rock analysis package with X-ray fluorescence (up to 19 laboratories depending on the element);
- Thermogravimetry: Loss on Ignition (LOI) at 1000 °C (12 laboratories used a thermogravimetric analyser, 4 laboratories included LOI with their fusion package and 3 laboratories used a conventional muffle furnace);
- Sodium peroxide/borate fusion with full suite ICP-OES and ICP-MS elemental packages (up to 15 laboratories depending on the element);
- Total C and S by infrared combustion furnace (20 laboratories).

For the round robin program twelve 300 g test units were taken at predetermined intervals during the bagging stage, immediately following homogenisation and are considered representative of the entire prepared batch. The six samples received by each laboratory were obtained by taking a 20 g subsample from six different 300 g test units (either from the odd or even numbered test units). Homogeneity was evaluated by submitting 12 x 20 g pulp samples to a single laboratory for XRF analysis. Paired samples were taken from each of the odd-numbered sampling units, allowing for an Analysis of Variance (ANOVA) to compare within- and between-unit variances across the six pairs. This statistical approach provides a relative measure of homogeneity and tests the null hypothesis that all sampling units originate from the same population distribution (see 'Homogeneity Evaluation' section below).

STATISTICAL ANALYSIS

Certified Values and their uncertainty intervals (Table 1) have been determined for each analyte following removal of individual, laboratory dataset (batch) and 3SD outliers (single iteration).

For individual outliers within a laboratory batch the z-score test is used in combination with a second method that determines the per cent deviation of the individual value from the batch median. Outliers in general are selected on the basis of z-scores > 2.5 and with per cent deviations (i) > 3 and (ii) more than three times the average absolute per cent deviation for the batch. Each laboratory data set mean is tested for outlying status based on z-score discrimination and rejected if > 2.5 . After individual and laboratory data set (batch) outliers have been eliminated a non-iterative 3 standard deviation filter is applied, with those values lying outside this window also relegated to outlying status. However, while statistics are taken into account, the exercise of a statistician's prerogative plays a significant role in identifying outliers.

95% Expanded Uncertainty provides a 95 % probability that the true value of the analyte under consideration lies between the upper and lower limits and is calculated according to the method outlined in [5] and [15]. All known or suspected sources of bias have been investigated or taken into account.

Indicative (uncertified) values (Table 2) are present where the number of laboratories reporting a particular analyte is insufficient (< 5) to support certification or where interlaboratory consensus is poor. This data is intended for 'informational purposes' only.

Standard Deviation intervals (see Table 5, 'Performance Gates') provide an indication of a level of performance that might reasonably be expected from a laboratory being monitored by this CRM in a QA/QC program. They take into account errors attributable to measurement uncertainty and CRM variability. For an effective CRM the contribution of the latter should be negligible in comparison to measurement errors. The Standard Deviation values include all sources of measurement uncertainty: between-lab variance, within-run variance (precision errors) and CRM variability.

The SD for each analyte's certified value is calculated from the same filtered data set used to determine the certified value, i.e., after removal of all individual, lab dataset (batch) and 3SD outliers (single iteration). These outliers can only be removed after the absolute homogeneity of the CRM has been independently established, i.e., the outliers must be confidently deemed to be analytical rather than arising from inhomogeneity of the CRM. ***The standard deviation is then calculated for each analyte from the pooled accepted analyses generated from the certification program.***

Homogeneity Evaluation

The tolerance limits (ISO 16269:2014) shown in Table 1 were determined using an analysis of precision errors method and are considered a conservative estimate of true homogeneity. The meaning of tolerance limits may be illustrated for nickel (Ni) by fusion XRF, where 99 % of the time ($1-\alpha=0.99$) at least 95 % of subsamples ($p=0.95$) will have concentrations lying between 0.514 and 0.526 wt.%. Put more precisely, this means that if the same number of subsamples were taken and analysed in the same manner repeatedly, 99 % of the tolerance intervals so constructed would cover at least 95 % of the total population, and 1 % of the tolerance intervals would cover less than 95 % of the total population. ***Please note that tolerance limits pertain to the homogeneity of the CRM only and should not be used as control limits for laboratory performance.***

Analysis of Variance (ANOVA) Study

In addition to the precision error method outlined above, homogeneity was also evaluated using an ANOVA study. This involved sending 12 x 20 g pulp samples to the BV Geoanalytical laboratory in Perth, Western Australia for analysis by borate fusion with XRF finish (code XRF201). The 12 samples consisted of paired samples from each of the odd numbered sampling units to enable an Analysis of Variance (ANOVA) by comparison of within- and between-unit variances across the six pairs. The ANOVA enables a relative measure of homogeneity and permits a test of the null hypothesis that all 'units' are drawn from the same population distribution. An ANOVA constructed in this way tests that no statistically significant difference exists in the variance between-units to that of the variance within-units. A p -value < 0.05 would indicate rejection of the null hypothesis at the 95 % confidence level (i.e., a significant difference likely does exist; meaning there is evidence of heterogeneity between the sample intervals).

All p -values were found to be statistically insignificant and the Null Hypothesis is therefore retained. It is important to note that ANOVA provides a relative measure of homogeneity and that a CRM having poor absolute homogeneity can still pass these tests if the within-unit heterogeneity is large and similar across all units. Based on the statistical analysis of the results of the interlaboratory certification program, it can be concluded that OREAS 181b is fit-for-purpose as a certified reference material (see 'Intended Use' below).

PERFORMANCE GATES

Table 5 below shows intervals calculated for two and three standard deviations. As a guide these intervals may be regarded as warning or rejection for multiple 2SD outliers, or rejection for individual 3SD outliers in QC monitoring, although their precise application should be at the discretion of the QC manager concerned (also see 'Intended Use' section below). Westgard Rules extend the basics of single-rule QC monitoring using multi-rules (for more information visit www.westgard.com/mltrule.htm). A second method utilises a 5 % window calculated directly from the certified value.

Standard deviation is also shown in relative percent for one, two and three relative standard deviations (1RSD, 2RSD and 3RSD) to facilitate an appreciation of the magnitude of these numbers and a comparison with the 5 % window. Caution should be exercised when concentration levels approach lower limits of detection of the analytical methods employed as performance gates calculated from standard deviations tend to be excessively wide whereas those determined by the 5 % method are too narrow. One approach used at commercial laboratories is to set the acceptance criteria at twice the detection level (DL) $\pm$ 10 %.

i.e., Certified Value $\pm$ 10 % $\pm$ 2DL [1].

Table 5. Performance Gates for OREAS 181b.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5 % window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
Borate Fusion XRF											
Al ₂ O ₃ , wt. %	7.20	0.095	7.01	7.39	6.91	7.48	1.32%	2.65%	3.97%	6.84	7.56
BaO, ppm	238	42	154	323	112	365	17.74%	35.48%	53.21%	226	250
CaO, wt. %	0.364	0.007	0.350	0.378	0.343	0.385	1.93%	3.85%	5.78%	0.346	0.382
Co, ppm	458	8	442	473	434	481	1.71%	3.42%	5.13%	435	481
Cr ₂ O ₃ , wt. %	0.657	0.014	0.629	0.684	0.616	0.698	2.09%	4.19%	6.28%	0.624	0.690
Cu, ppm	< 50	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Fe ₂ O ₃ , wt. %	34.61	0.324	33.96	35.26	33.64	35.58	0.94%	1.87%	2.81%	32.88	36.34
K ₂ O, wt. %	0.733	0.012	0.710	0.756	0.698	0.768	1.59%	3.19%	4.78%	0.696	0.770
MgO, wt. %	5.77	0.074	5.63	5.92	5.55	6.00	1.28%	2.57%	3.85%	5.49	6.06
MnO, wt. %	0.174	0.006	0.163	0.185	0.158	0.191	3.17%	6.33%	9.50%	0.166	0.183
Na ₂ O, wt. %	0.330	0.026	0.277	0.382	0.251	0.408	7.92%	15.84%	23.77%	0.313	0.346
Ni, wt. %	0.520	0.014	0.492	0.548	0.477	0.562	2.72%	5.45%	8.17%	0.494	0.546
P ₂ O ₅ , wt. %	0.035	0.004	0.026	0.044	0.022	0.049	12.70%	25.40%	38.10%	0.034	0.037
SiO ₂ , wt. %	38.83	0.379	38.07	39.59	37.69	39.97	0.98%	1.95%	2.93%	36.89	40.77
Sn, ppm	< 50	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
SO ₃ , wt. %	0.267	0.020	0.228	0.307	0.208	0.327	7.46%	14.92%	22.38%	0.254	0.281
TiO ₂ , wt. %	0.332	0.010	0.312	0.353	0.302	0.363	3.09%	6.18%	9.27%	0.316	0.349
V ₂ O ₅ , ppm	165	29	108	223	79	252	17.47%	34.93%	52.40%	157	174
Zn, ppm	92	14	63	121	49	135	15.59%	31.18%	46.78%	87	97
Thermogravimetry											
LOI ¹⁰⁰⁰ , wt. %	9.78	0.239	9.30	10.26	9.06	10.50	2.45%	4.89%	7.34%	9.29	10.27
Borate / Peroxide Fusion ICP											
Al, wt. %	3.74	0.054	3.63	3.85	3.58	3.90	1.43%	2.87%	4.30%	3.55	3.93

SI unit equivalents: ppm (parts per million; 1×10^{-6}) $\equiv$ mg/kg; wt. % (weight per cent) $\equiv$ % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding; IND = indeterminate.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Table 5 continued.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5 % window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
Borate / Peroxide Fusion ICP continued											
As, ppm	115	16	83	147	67	162	13.77%	27.55%	41.32%	109	121
B, ppm	354	42	269	439	227	482	11.97%	23.95%	35.92%	337	372
Ba, ppm	210	6	199	222	193	227	2.70%	5.40%	8.09%	200	221
Be, ppm	1.07	0.096	0.88	1.26	0.78	1.36	9.00%	18.00%	27.00%	1.02	1.12
Bi, ppm	4.89	0.94	3.00	6.78	2.06	7.72	19.29%	38.59%	57.88%	4.65	5.13
Ca, wt. %	0.258	0.037	0.184	0.331	0.147	0.368	14.31%	28.61%	42.92%	0.245	0.270
Cd, ppm	< 10	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Ce, ppm	34.1	3.6	26.8	41.4	23.1	45.0	10.70%	21.40%	32.10%	32.4	35.8
Co, ppm	442	21	401	483	380	504	4.66%	9.33%	13.99%	420	464
Cr, wt. %	0.445	0.011	0.423	0.468	0.411	0.479	2.53%	5.06%	7.59%	0.423	0.467
Cs, ppm	2.68	0.190	2.30	3.06	2.11	3.25	7.11%	14.23%	21.34%	2.54	2.81
Cu, ppm	40.7	2.09	36.6	44.9	34.5	47.0	5.14%	10.28%	15.42%	38.7	42.8
Dy, ppm	2.08	0.203	1.67	2.49	1.47	2.69	9.75%	19.49%	29.24%	1.98	2.18
Er, ppm	1.16	0.091	0.98	1.35	0.89	1.44	7.84%	15.69%	23.53%	1.10	1.22
Eu, ppm	0.54	0.07	0.41	0.67	0.35	0.74	12.09%	24.19%	36.28%	0.51	0.57
Fe, wt. %	24.12	0.441	23.23	25.00	22.79	25.44	1.83%	3.66%	5.49%	22.91	25.32
Ga, ppm	9.38	0.682	8.02	10.75	7.34	11.43	7.27%	14.54%	21.81%	8.91	9.85
Gd, ppm	2.07	0.23	1.62	2.53	1.39	2.75	10.96%	21.92%	32.89%	1.97	2.18
Ge, ppm	1.78	0.35	1.08	2.48	0.73	2.83	19.59%	39.17%	58.76%	1.69	1.87
Ho, ppm	0.40	0.021	0.35	0.44	0.33	0.46	5.38%	10.75%	16.13%	0.38	0.42
In, ppm	< 0.1	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
K, wt. %	0.626	0.056	0.514	0.738	0.458	0.794	8.94%	17.88%	26.82%	0.595	0.658
La, ppm	13.7	1.16	11.4	16.0	10.2	17.2	8.45%	16.90%	25.34%	13.0	14.4
Li, ppm	12.7	3.5	5.6	19.8	2.1	23.3	27.78%	55.56%	83.34%	12.1	13.3
Lu, ppm	0.16	0.03	0.10	0.21	0.07	0.24	17.58%	35.16%	52.73%	0.15	0.16
Mg, wt. %	3.40	0.089	3.22	3.57	3.13	3.66	2.61%	5.22%	7.83%	3.23	3.57
Mn, wt. %	0.134	0.003	0.127	0.141	0.124	0.145	2.58%	5.17%	7.75%	0.128	0.141
Mo, ppm	2.37	0.52	1.33	3.42	0.80	3.94	22.07%	44.14%	66.20%	2.25	2.49
Nd, ppm	11.2	0.68	9.8	12.5	9.1	13.2	6.09%	12.19%	18.28%	10.6	11.7
Ni, wt. %	0.513	0.012	0.489	0.536	0.477	0.548	2.32%	4.65%	6.97%	0.487	0.538
Pr, ppm	3.17	0.315	2.54	3.80	2.23	4.12	9.93%	19.85%	29.78%	3.01	3.33
Rb, ppm	33.4	1.81	29.8	37.0	28.0	38.8	5.41%	10.81%	16.22%	31.8	35.1
Re, ppm	< 0.1	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
S, wt. %	0.097	0.018	0.061	0.134	0.042	0.152	18.83%	37.65%	56.48%	0.093	0.102
Sc, ppm	19.8	0.92	17.9	21.6	17.0	22.5	4.65%	9.30%	13.95%	18.8	20.8
Se, ppm	< 20	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Si, wt. %	18.04	0.361	17.32	18.76	16.96	19.12	2.00%	4.00%	6.00%	17.14	18.94
Sm, ppm	2.28	0.31	1.67	2.89	1.36	3.20	13.44%	26.89%	40.33%	2.17	2.39
Sr, ppm	32.5	2.80	26.9	38.1	24.1	40.9	8.60%	17.21%	25.81%	30.9	34.1
Tb, ppm	0.33	0.05	0.23	0.43	0.18	0.48	15.38%	30.77%	46.15%	0.31	0.34
Te, ppm	< 1	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Th, ppm	4.62	0.50	3.63	5.62	3.14	6.11	10.72%	21.43%	32.15%	4.39	4.86
Ti, wt. %	0.196	0.006	0.183	0.209	0.177	0.215	3.25%	6.50%	9.75%	0.186	0.206

SI unit equivalents: ppm (parts per million; 1×10^{-6}) $\equiv$ mg/kg; wt. % (weight per cent) $\equiv$ % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding; IND = indeterminate.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Table 5 continued.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5 % window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
Borate / Peroxide Fusion ICP continued											
Tl, ppm	< 0.5	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Tm, ppm	0.17	0.014	0.14	0.20	0.13	0.21	8.15%	16.29%	24.44%	0.16	0.18
U, ppm	1.02	0.16	0.71	1.34	0.55	1.50	15.44%	30.88%	46.32%	0.97	1.07
V, ppm	85	6.6	71	98	65	104	7.84%	15.69%	23.53%	80	89
W, ppm	22.9	3.0	17.0	28.9	14.1	31.8	12.91%	25.82%	38.73%	21.8	24.1
Y, ppm	10.5	0.61	9.2	11.7	8.6	12.3	5.84%	11.68%	17.51%	9.9	11.0
Yb, ppm	1.15	0.098	0.95	1.35	0.86	1.44	8.49%	16.99%	25.48%	1.09	1.21
Zn, ppm	95	7.1	81	110	74	117	7.47%	14.95%	22.42%	91	100
Infrared Combustion											
C, wt. %	1.10	0.029	1.04	1.15	1.01	1.18	2.66%	5.32%	7.98%	1.04	1.15
S, wt. %	0.102	0.009	0.084	0.120	0.075	0.129	8.95%	17.91%	26.86%	0.097	0.107

SI unit equivalents: ppm (parts per million; 1×10^{-6}) $\equiv$ mg/kg; wt. % (weight per cent) $\equiv$ % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding; IND = indeterminate.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

PARTICIPATING LABORATORIES

1. Actlabs, Ancaster, Ontario, Canada
2. ALS, Brisbane, QLD, Australia
3. ALS, Lima, Peru
4. ALS, Loughrea, Galway, Ireland
5. American Assay Laboratories, Sparks, Nevada, USA
6. ARGETEST Mineral Processing, Ankara, Central Anatolia, Turkey
7. Bureau Veritas Commodities Canada Ltd, Vancouver, BC, Canada
8. Bureau Veritas Geoanalytical, Adelaide, SA, Australia
9. Bureau Veritas Geoanalytical, Perth, WA, Australia
10. Bureau Veritas Minerals, Ankara, Central Anatolia, Turkey
11. CERTIMIN, Lima, Peru
12. Inspectorate (BV), Lima, Peru
13. Inspectorate Griffith India, Gandhidham, Gujarat, India
14. Intertek, Cupang, Muntinlupa, Philippines
15. Intertek, Perth, WA, Australia
16. Labwest Minerals Analysis, Perth, WA, Australia
17. MSALABS, Vancouver, BC, Canada
18. Ni Lab, Pouembout, New Caledonia
19. Paragon Geochemical Laboratories, Sparks, Nevada, USA
20. PT Geoservices Ltd, Cikarang, Jakarta Raya, Indonesia
21. PT Intertek Utama Services, Jakarta Timur, DKI Jakarta, Indonesia
22. SGS Australia Mineral Services, Perth, WA, Australia
23. SGS Canada Inc., Vancouver, BC, Canada
24. Shiva Analyticals Ltd, Bangalore North, Karnataka, India
25. Skyline Assayers & Laboratories, Tucson, Arizona, USA
26. Stewart Assay & Environmental Laboratories LLC, Kara-Balta, Chüy, Kyrgyzstan

Please note: To preserve anonymity, the above numbered alphabetical list of participating laboratories does not correspond with the Lab ID numbering on the scatter plots below.

Figure 1. Ni by Borate Fusion XRF in OREAS 181b


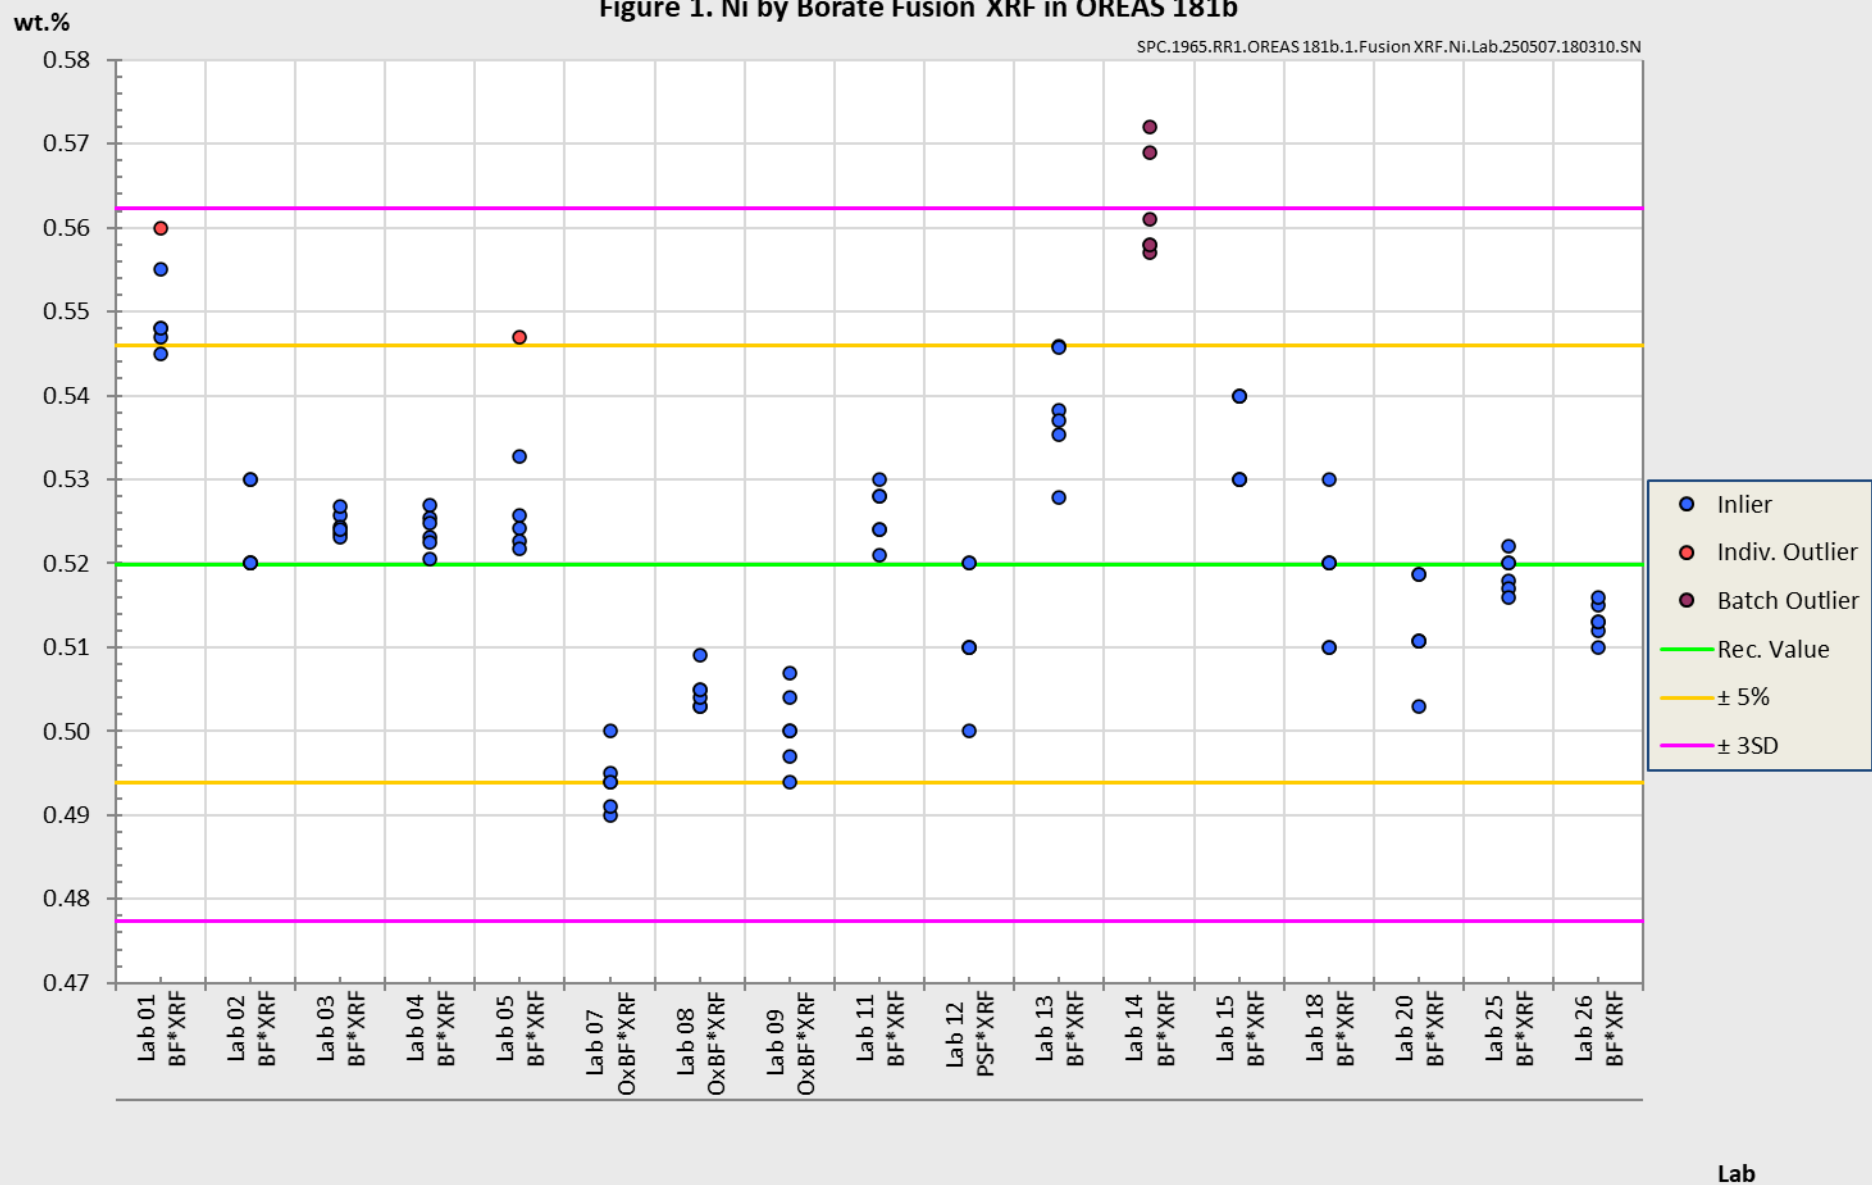


Figure 2. Co by Borate Fusion XRF in OREAS 181b

SPC.1965.RR1.OREAS 181b.1.Fusion XRF.Co.Lab.250507.180141.SN

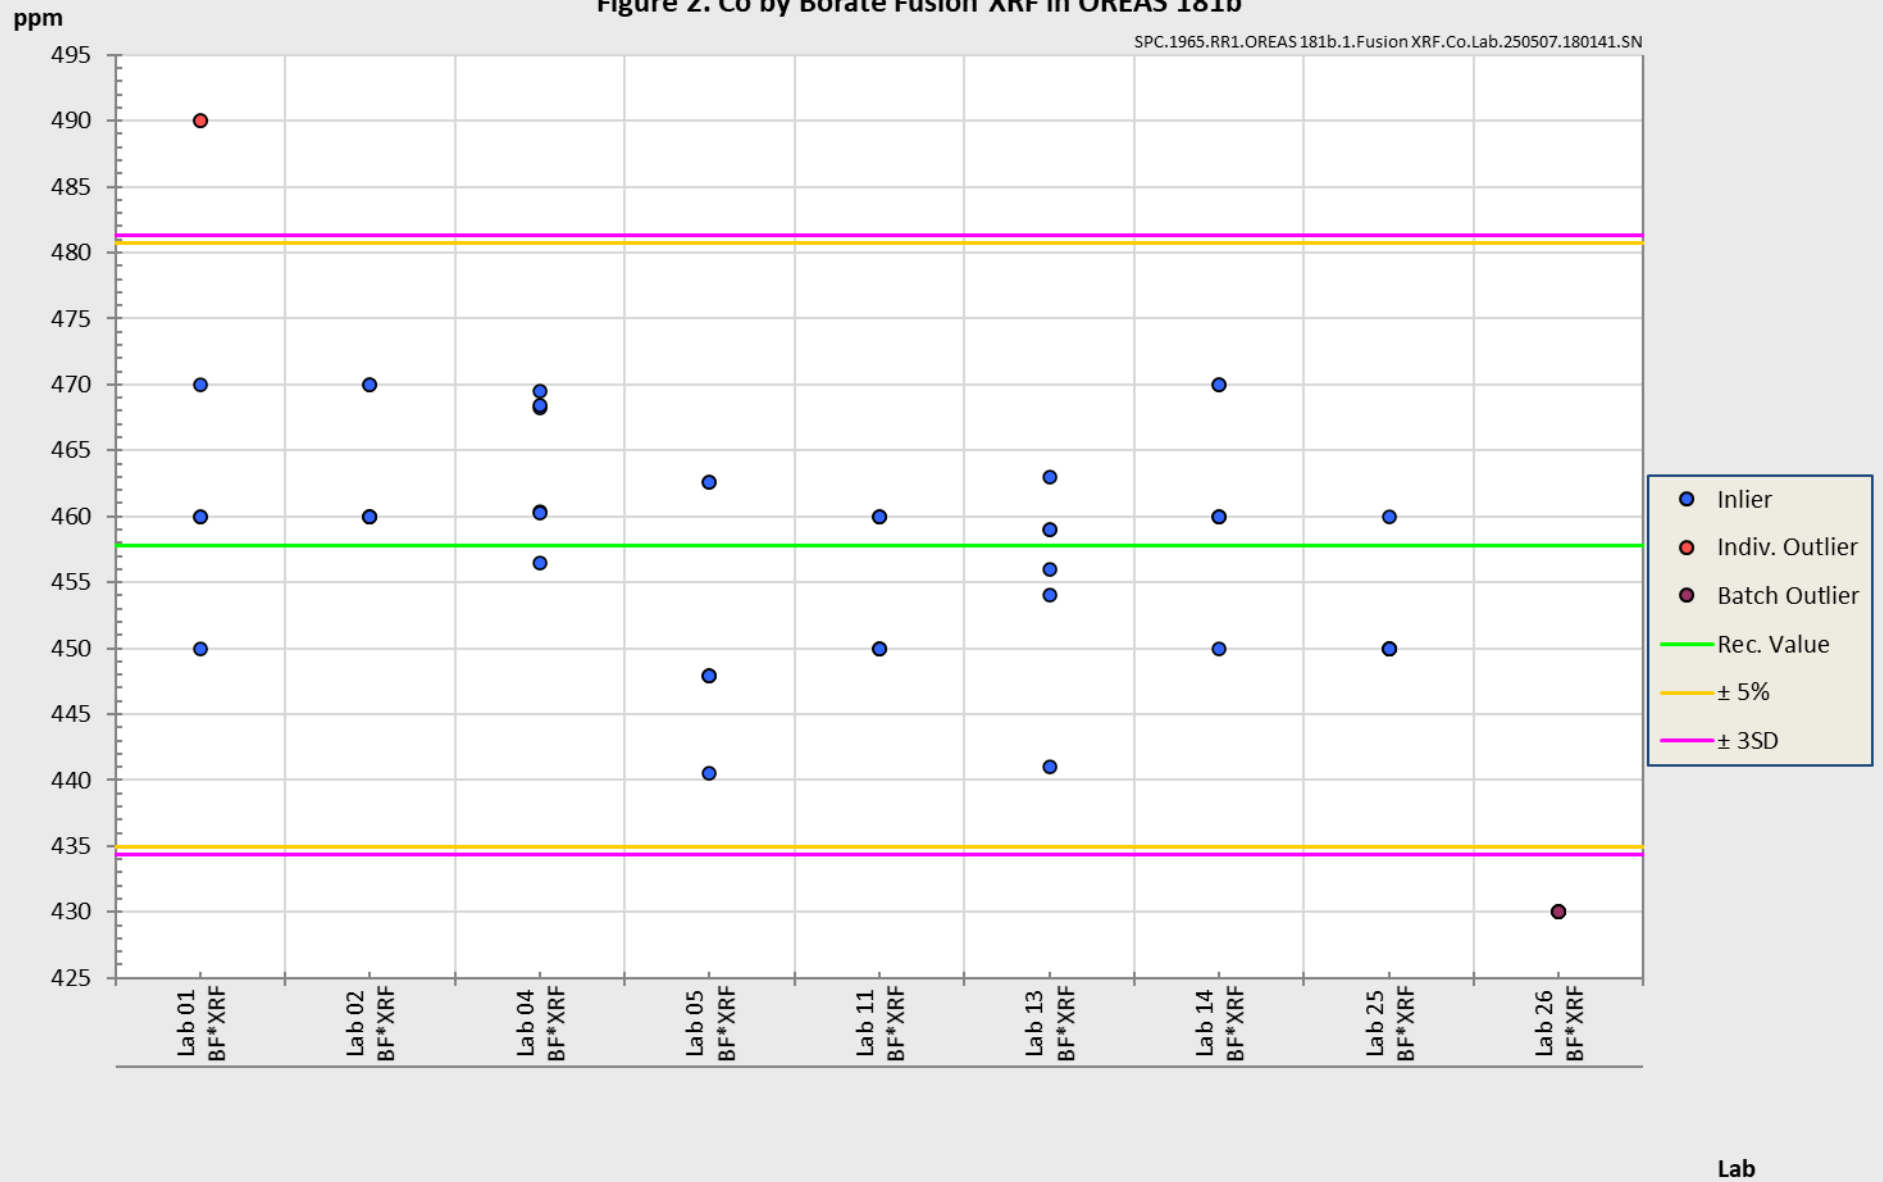

PREPARER AND SUPPLIER

Certified reference material OREAS 181b is prepared, certified and supplied by:

ORE Research & Exploration Pty Ltd	Tel: +613-9729 0333
37A Hosie Street	Web: www.oreas.com
Bayswater North VIC 3153	Email: info@ore.com.au
AUSTRALIA	

METROLOGICAL TRACEABILITY

The interlaboratory results that underpin the certified values are metrologically traceable to the international measurement scale (SI) of mass (either as a % mass fraction or as milligrams per kilogram (mg/kg)) [14]. In line with popular use, all data within tables in this certificate are expressed as the mass fraction in either weight percent (wt.%) or parts per million (ppm).

The analytical samples sent to participating laboratories were selected in a manner to be representative of the entire prepared batch of CRM. This representativeness was maintained in each submitted laboratory sample batch and ensures the user that the data is traceable from sample selection through to the analytical results. The systematic sampling method was chosen due to the low risk of overlooking repetitive effects or trends in the batch due to the way the CRM was processed. In line with ISO 17025 [8], each analytical data set received from the participating laboratories has been validated by its assayer through the inclusion of internal reference materials and QC checks during and post analysis.

The participating laboratories were chosen on the basis of their competence (from past performance in interlaboratory programs undertaken by ORE Pty Ltd) for a particular analytical method, analyte or analyte suite and sample matrix. These laboratories are accredited to ISO 17025 for all methods (Table 1). The certified values presented in this report are calculated from the means of accepted data following robust technical and statistical analysis as detailed in this report.

Guide ISO/TR 16476:2016 [7], section 5.3.1 describes metrological traceability in reference materials as it pertains to the transformation of the measurand. In this section it states, *“Although the determination of the property value itself can be made traceable to appropriate units through, for example, calibration of the measurement equipment used, steps like the transformation of the sample from one physical (chemical) state to another cannot. Such transformations may only be compared with a reference (when available), or among themselves. For some transformations, reference methods have been defined and may be used in certification projects to evaluate the uncertainty associated with such a transformation. In other cases, only a comparison among different laboratories using the same procedure is possible. In this case, it is impossible to demonstrate absence of method bias; therefore, the result is an operationally defined measurand (ISO 33405:2024-05, 9.2.4c) [4].”* Certification takes place on the basis of agreement among operationally defined, independent measurement results.

COMMUTABILITY

The measurements of the results that underlie the certified values contained in this report were undertaken by methods involving pre-treatment (fusion/digestion) of the sample. This served to reduce the sample to a simple and well understood form permitting calibration using simple solutions of the CRM. Due to these methods being well understood and highly effective, commutability is not an issue for this CRM. All OREAS CRMs are sourced from natural ore minerals meaning they will display similar behaviour as routine 'field' samples in the relevant measurement process. Care should be taken to ensure 'matrix matching' as close as practically achievable. The matrix and mineralisation style of the CRM is described in the 'Source Material' section and users should select appropriate CRMs matching these attributes to the field samples being analysed.

INTENDED USE

OREAS 181b is intended to cover all activities needed to produce a measurement result. This includes extraction, possible separation steps and the actual measurement process (the signal producing step). OREAS 181b may be used to calibrate the entire procedure by producing a pure substance CRM transformed into a calibration solution.

OREAS 181b is intended for the following uses:

- For the monitoring of laboratory performance in the analysis of analytes reported in Table 1 geological samples;
- For the verification/ validation of analytical methods for analytes reported in Table 1;
- For the calibration of instruments used in the determination of the concentration of analytes reported in Table 1. When a value provided in this certificate is used to calibrate a measurement process, the uncertainty associated with that value should be appropriately propagated into the user's uncertainty calculation. Users can determine an approximation of the standard uncertainty by calculating one fourth of the width of the Expanded Uncertainty interval given in this certificate (Expanded Uncertainty intervals are provided in Table 1).

MINIMUM SAMPLE SIZE

To relate analytical determinations to the values in this certificate, the minimum mass of sample used should match the typical mass that the laboratories used in the interlaboratory (round robin) certification program. This means that different minimum sample masses should be used depending on the operationally defined methodology as follows:

- Borate fusion with X-ray fluorescence finish: ≥ 0.2 g;
- Loss on Ignition (LOI) at 1000 °C: ≥ 1 g;
- Sodium peroxide / Lithium Borate fusion with ICP-OES and/or MS finish: ≥ 0.2 g;
- Total C and S by infrared combustion furnace: ≥ 0.1 g.

PERIOD OF VALIDITY & STORAGE INSTRUCTIONS

The certification of OREAS 181b remains valid, within the specified measurement uncertainties, until at least July 2039, provided the CRM is handled and stored in accordance

with the instructions given below. This certification is nullified if the CRM is any way changed or contaminated.

Store in a clean and cool dry place away from direct sunlight.

Long-term stability will be monitored at appropriate intervals and purchasers notified if any changes are observed. The period of validity may well be indefinite and will be reassessed prior to expiry with the aim of extending the validity if possible.

Single-use sachets

OREAS 181b is packaged in single-use laminated foil sachets. Following analysis, it is the manufacturer's expectation that any remaining material is discarded. It is the user's responsibility to prevent contamination and avoid prolonged exposure of the sample to the atmosphere prior to analysis.

Repeat-use packaging (e.g., 500 g plastic jars)

After taking a subsample, users should replace the lid of the jar promptly and securely to prevent accidental spills and airborne contamination. OREAS 181b contains a pre-equilibrated hygroscopic* matrix with an indicative value for moisture provided to enable users to check for changes to stored material by determining moisture in the user's laboratory and comparing the result to the value in Table 3 in this certificate.

The stability of the CRM in regard to oxidation from the breakdown of sulphide minerals to sulphates is negligible given its low sulphur concentration (~0.10 wt.% S).

*A pre-equilibrated hygroscopic matrix means exposure to atmospheres significantly different, in terms of temperature and humidity, from the climate during manufacturing should have negligible impact on the precision of results. Hygroscopic moisture is the amount of adsorbed moisture (weakly held H₂O- molecules on the surface of exposed material) following exposure to the local atmosphere. Usually, equilibration of material to the local atmosphere will occur if the material is spread into a thin (~2mm thick) layer and left exposed for a period of 2 hours.

INSTRUCTIONS FOR HANDLING & CORRECT USE

Pre-homogenisation of the CRM prior to subsampling and analysis is not necessary as there is no particle segregation under transport [12].

Fine powders pose a risk to eyes and lungs and therefore standard precautions including the use of safety glasses and dust masks are advised.

As per routine analysis at commercial laboratories, the certified values derived by borate fusion with XRF finish are on a dry sample basis.

Analytes by all other methods refer to the concentration levels in the packaged state. There is no need for drying prior to weighing and analysis for these methods.

QC monitoring using multiples of the Standard Deviation (SD)

In the application of SD's in monitoring performance it is important to note that not all laboratories function at the same level of proficiency and that different methods in use at a particular laboratory have differing levels of precision. Each laboratory has its own inherent

SD (for a specific concentration level and analyte-method pair) based on the analytical process and this SD is not directly related to the round robin program.

The majority of data generated in the round robin program was produced by a selection of world class laboratories. The SD's thus generated are more constrained than those that would be produced across a randomly selected group of laboratories. To produce more generally achievable SD's the 'pooled' SD's provided in this report include interlaboratory bias. This 'one size fits all' approach may require revision at the discretion of the QC manager concerned following careful scrutiny of QC control charts.

The performance gates shown in Table 5 are intended only to be used as a preliminary guide as to what a laboratory may be able to achieve. Over a period of time monitoring your own laboratory's data for this CRM, SD's should be calculated directly from your own laboratory's process. This will enable you to establish more specific performance gates that are fit for purpose for your application as well as the ability to monitor bias. If your long-term trend analysis shows an average value that is within the 95 % expanded uncertainty then generally there is no cause for concern in regard to bias.

LEGAL NOTICE

Ore Research & Exploration Pty Ltd has prepared and statistically evaluated the property values of this reference material to the best of its ability. The Purchaser by receipt hereof releases and indemnifies Ore Research & Exploration Pty Ltd from and against all liability and costs arising from the use of this material and information.

© COPYRIGHT Ore Research & Exploration Pty Ltd.
Unauthorised copying, reproduction, storage or dissemination is prohibited.

CERTIFYING OFFICER

Craig Hamlyn (B.Sc. Hons - Geology), Technical Manager - ORE P/L

QMS CERTIFICATION

ORE Pty Ltd is accredited for compliance with ISO 17034:2016 (Accreditation number 20483).



ORE Pty Ltd is ISO 9001:2015 certified by Lloyd's Register Quality Assurance Ltd for its quality management system including development, manufacturing, certification and supply of CRMs.



DOCUMENT HISTORY

Revision No.	Date	Changes applied
1	14 th Aug, 2025	Converted Fe and Mg to their oxide forms for Borate Fusion XRF.
0	27 th May, 2025	First publication.

REFERENCES

- [1] Govett, G.J.S. (1983). Handbook of Exploration Geochemistry, Volume 2: Statistics and Data Analysis in Geochemical Prospecting (Variations of accuracy and precision).
- [2] ISO Guide 30:2015. Terms and definitions used in connection with reference materials.
- [3] ISO 33401:2024-01. Reference materials – Contents of certificates, labels and accompanying documentation.
- [4] ISO 33405:2024-05. Reference materials – Approaches for characterization and assessment of homogeneity and stability.
- [5] ISO Guide 98-3:2008. Guide to the expression of uncertainty in measurement (GUM:1995).
- [6] ISO 16269:2014. Statistical interpretation of data – Part 6: Determination of statistical tolerance intervals.
- [7] ISO/TR 16476:2016, Reference Materials – Establishing and expressing metrological traceability of quantity values assigned to reference materials.
- [8] ISO 17025:2017, General requirements for the competence of testing and calibration laboratories.
- [9] ISO 17034:2016. General requirements for the competence of reference material producers.
- [10] Munsell Rock Color Book (2014). Rock-Color Chart Committee, Geological Society of America (GSA), Minnesota (USA).
- [11] OREAS-BUP-70-09-11: Statistical Analysis - OREAS Evaluation Method.
- [12] OREAS-TN-04-1498: Stability under transport; an experimental study of OREAS CRMs.
- [13] OREAS-TN-05-1674: Long-term storage stability; an experimental study of OREAS CRMs.
- [14] Thompson, A.; Taylor, B.N. (2008); Guide for the Use of the International System of Units (SI); NIST Special Publication 811; U.S. Government Printing Office: Washington, DC; available at: <https://physics.nist.gov/cuu/pdf/sp811.pdf> (accessed Nov 2021).
- [15] Van der Veen A.M.H. et al. (2001). Uncertainty calculations in the certification of reference materials, Accred Qual Assur 6: 290-294.