

CERTIFICATE OF ANALYSIS FOR


CERTIFIED REFERENCE MATERIAL

OREAS 911

**Volcanogenic Massive Sulphide (VMS) Au-Cu-Ag-Zn Ore
Newfoundland & Labrador, Canada**



Accredited for compliance with ISO 17034



COA-1941-OREAS 911-R0	01-Apr-2026
Template ID: BUP-70-10-03 Ver:1.0	

Table 1. Certified Values, Uncertainty & Tolerance Intervals in OREAS 911.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
Pb Fire Assay					
Au, Gold (ppm)	0.762	0.748	0.776	0.759*	0.765*
Aqua Regia Digestion (sample weights 15-50g)					
Au, Gold (ppm)	0.750	0.730	0.770	0.747*	0.753*
Infrared Combustion					
S, Sulphur (wt.%)	11.00	10.74	11.25	10.88	11.11
Borate / Peroxide Fusion ICP					
Al, Aluminium (wt.%)	6.19	6.06	6.32	6.09	6.29
As, Arsenic (ppm)	477	453	502	462	493
Ba, Barium (ppm)	1717	1654	1780	1681	1753
Be, Beryllium (ppm)	1.90	1.57	2.24	1.69	2.12
Bi, Bismuth (ppm)	2.31	2.07	2.55	2.17	2.45
Ca, Calcium (wt.%)	1.27	1.21	1.34	1.23	1.31
Cd, Cadmium (ppm)	19.7	18.2	21.2	18.7	20.6
Ce, Cerium (ppm)	56	53	58	54	58
Co, Cobalt (ppm)	35.8	33.4	38.2	34.4	37.2
Cr, Chromium (ppm)	57	50	64	53	61
Cs, Caesium (ppm)	3.76	3.40	4.11	3.55	3.97
Cu, Copper (wt.%)	0.506	0.490	0.522	0.498	0.515
Dy, Dysprosium (ppm)	2.48	2.24	2.72	2.37	2.60
Er, Erbium (ppm)	0.84	0.71	0.97	0.78	0.89
Eu, Europium (ppm)	0.91	0.76	1.07	0.87	0.95
Fe, Iron (wt.%)	11.64	11.37	11.92	11.42	11.86
Ga, Gallium (ppm)	18.3	16.7	19.9	17.6	19.1
Gd, Gadolinium (ppm)	3.80	3.50	4.10	3.66	3.94
Ge, Germanium (ppm)	2.71	2.30	3.12	2.46	2.96
Hf, Hafnium (ppm)	4.63	4.07	5.19	IND	IND
Ho, Holmium (ppm)	0.38	0.32	0.44	0.35	0.40
In, Indium (ppm)	0.65	0.56	0.74	IND	IND
K, Potassium (wt.%)	2.36	2.27	2.44	2.30	2.42
La, Lanthanum (ppm)	27.9	26.3	29.5	27.1	28.7
Li, Lithium (ppm)	16.3	12.8	19.8	13.1	19.5
Lu, Lutetium (ppm)	0.076	0.059	0.092	IND	IND
Mg, Magnesium (wt.%)	0.400	0.384	0.416	0.390	0.410
Mn, Manganese (wt.%)	0.031	0.030	0.032	0.030	0.032
Nb, Niobium (ppm)	11.7	10.7	12.6	11.2	12.2
Nd, Neodymium (ppm)	24.1	22.9	25.4	23.1	25.1
Ni, Nickel (ppm)	25.1	17.0	33.2	21.0	29.1
P, Phosphorus (wt.%)	0.023	0.019	0.026	0.021	0.025
Pb, Lead (ppm)	614	579	648	595	633

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

*Gold Tolerance Limits for typical 30 g fire assay and 25 g aqua regia digestion methods are determined from 20 x 85 mg INAA results and the Sampling Constant (Ingamells & Switzer, 1973).

Note: intervals may appear asymmetric due to rounding.

IND = indeterminate (due to limited reading resolution of the methods employed).

Table 1 continued.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
Borate / Peroxide Fusion ICP continued					
Pr, Praseodymium (ppm)	6.50	6.14	6.86	6.36	6.64
Rb, Rubidium (ppm)	94	89	98	90	97
S, Sulphur (wt.%)	11.03	10.75	11.31	10.88	11.18
Sb, Antimony (ppm)	49.1	46.0	52.2	46.7	51.4
Sc, Scandium (ppm)	< 10	IND	IND	IND	IND
Se, Selenium (ppm)	25.7	15.7	35.7	22.9	28.6
SiO ₂ , Silicon dioxide (wt.%)	54.71	53.40	56.03	53.88	55.55
Sm, Samarium (ppm)	4.66	4.31	5.02	4.50	4.82
Sn, Tin (ppm)	8.31	6.58	10.04	IND	IND
Sr, Strontium (ppm)	129	121	136	124	133
Ta, Tantalum (ppm)	0.93	0.70	1.16	0.87	0.99
Tb, Terbium (ppm)	0.51	0.45	0.58	0.48	0.55
Te, Tellurium (ppm)	2.20	1.13	3.27	IND	IND
Th, Thorium (ppm)	8.79	8.37	9.22	8.62	8.97
Ti, Titanium (wt.%)	0.135	0.129	0.142	0.131	0.140
Tl, Thallium (ppm)	5.00	4.70	5.31	4.81	5.19
Tm, Thulium (ppm)	0.098	0.079	0.117	IND	IND
U, Uranium (ppm)	5.30	4.98	5.63	5.10	5.51
V, Vanadium (ppm)	43.8	41.1	46.6	42.5	45.2
W, Tungsten (ppm)	3.42	2.27	4.57	2.85	3.99
Y, Yttrium (ppm)	11.3	10.6	11.9	10.9	11.6
Yb, Ytterbium (ppm)	0.60	0.47	0.73	0.54	0.66
Zn, Zinc (wt.%)	0.497	0.481	0.513	0.488	0.507
Zr, Zirconium (ppm)	179	161	198	172	186
4-Acid Digestion					
Ag, Silver (ppm)	4.70	4.50	4.90	4.56	4.84
Al, Aluminium (wt.%)	6.03	5.85	6.20	5.89	6.17
As, Arsenic (ppm)	463	447	478	454	471
Be, Beryllium (ppm)	1.87	1.78	1.95	1.80	1.94
Bi, Bismuth (ppm)	2.41	2.30	2.53	2.35	2.48
Ca, Calcium (wt.%)	1.26	1.22	1.29	1.23	1.28
Cd, Cadmium (ppm)	20.7	19.9	21.4	20.2	21.1
Ce, Cerium (ppm)	51	48	54	49	53
Co, Cobalt (ppm)	36.6	35.5	37.8	35.9	37.4
Cr, Chromium (ppm)	46.8	43.6	50.0	44.9	48.7
Cs, Caesium (ppm)	3.70	3.50	3.90	3.59	3.82
Cu, Copper (wt.%)	0.496	0.482	0.510	0.488	0.504
Dy, Dysprosium (ppm)	2.41	2.23	2.59	2.33	2.49
Er, Erbium (ppm)	0.80	0.74	0.87	0.78	0.83
Eu, Europium (ppm)	0.87	0.83	0.92	0.84	0.90

SI unit equivalents: ppm (parts per million; $1 \times 10^{-6} \equiv \text{mg/kg}$; wt.% (weight per cent) $\equiv \%$ (mass fraction).

Note: intervals may appear asymmetric due to rounding.

IND = indeterminate (due to limited reading resolution of the methods employed. For practical purposes the 95% Expanded Uncertainty can be set between zero and a two times multiple of the upper bound/non-detect limit value).

Table 1 continued.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
4-Acid Digestion continued					
Fe, Iron (wt.%)	11.42	11.14	11.71	11.24	11.60
Ga, Gallium (ppm)	18.5	17.6	19.3	18.0	18.9
Gd, Gadolinium (ppm)	3.75	3.52	3.98	3.63	3.87
Ge, Germanium (ppm)	0.25	0.18	0.32	0.22	0.28
Hf, Hafnium (ppm)	4.55	4.30	4.80	4.37	4.73
Ho, Holmium (ppm)	0.35	0.32	0.39	0.34	0.37
In, Indium (ppm)	0.67	0.63	0.71	0.64	0.69
K, Potassium (wt.%)	2.31	2.25	2.38	2.26	2.37
La, Lanthanum (ppm)	23.4	21.6	25.2	22.5	24.3
Li, Lithium (ppm)	15.0	14.3	15.8	14.6	15.5
Lu, Lutetium (ppm)	0.077	0.066	0.089	IND	IND
Mg, Magnesium (wt.%)	0.378	0.366	0.389	0.368	0.387
Mn, Manganese (wt.%)	0.031	0.030	0.031	0.030	0.031
Mo, Molybdenum (ppm)	30.0	28.8	31.3	29.4	30.7
Na, Sodium (wt.%)	1.72	1.67	1.76	1.69	1.75
Nb, Niobium (ppm)	11.5	11.0	11.9	11.1	11.8
Nd, Neodymium (ppm)	23.3	21.8	24.9	22.8	23.8
Ni, Nickel (ppm)	20.5	19.4	21.5	19.8	21.1
P, Phosphorus (wt.%)	0.020	0.019	0.021	0.019	0.021
Pb, Lead (ppm)	601	581	620	590	611
Pr, Praseodymium (ppm)	6.09	5.76	6.43	5.91	6.28
Rb, Rubidium (ppm)	91	87	95	89	93
Re, Rhenium (ppm)	0.008	0.006	0.010	IND	IND
S, Sulphur (wt.%)	10.48	10.07	10.89	10.35	10.61
Sb, Antimony (ppm)	47.3	44.9	49.7	45.4	49.2
Sc, Scandium (ppm)	8.21	7.77	8.65	7.89	8.53
Se, Selenium (ppm)	25.3	23.3	27.3	24.1	26.5
Sm, Samarium (ppm)	4.50	4.11	4.88	4.32	4.67
Sn, Tin (ppm)	7.67	7.30	8.04	7.35	7.99
Sr, Strontium (ppm)	118	113	123	116	120
Ta, Tantalum (ppm)	0.83	0.78	0.88	0.78	0.89
Tb, Terbium (ppm)	0.51	0.47	0.56	0.48	0.55
Te, Tellurium (ppm)	2.19	2.01	2.37	2.08	2.31
Th, Thorium (ppm)	7.79	7.16	8.42	7.53	8.04
Ti, Titanium (wt.%)	0.112	0.108	0.115	0.110	0.113
Tl, Thallium (ppm)	4.96	4.73	5.20	4.82	5.10
Tm, Thulium (ppm)	0.089	0.074	0.104	IND	IND
U, Uranium (ppm)	5.16	4.93	5.40	5.06	5.27
V, Vanadium (ppm)	43.9	42.1	45.7	42.7	45.1
W, Tungsten (ppm)	3.19	3.00	3.39	3.07	3.32
Y, Yttrium (ppm)	11.1	10.6	11.5	10.8	11.4

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

Note: intervals may appear asymmetric due to rounding.

IND = indeterminate (due to limited reading resolution of the methods employed).

Table 1 continued.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
4-Acid Digestion continued					
Yb, Ytterbium (ppm)	0.57	0.52	0.62	0.54	0.60
Zn, Zinc (wt.%)	0.494	0.479	0.509	0.487	0.501
Zr, Zirconium (ppm)	170	164	176	167	173
Aqua Regia Digestion					
Ag, Silver (ppm)	4.80	4.59	5.01	4.65	4.95
Al, Aluminium (wt.%)	0.753	0.717	0.789	0.733	0.773
As, Arsenic (ppm)	459	446	472	452	465
B, Boron (ppm)	< 10	IND	IND	IND	IND
Be, Beryllium (ppm)	0.29	0.27	0.31	0.27	0.31
Bi, Bismuth (ppm)	2.37	2.24	2.49	2.25	2.48
Ca, Calcium (wt.%)	0.714	0.685	0.744	0.701	0.727
Cd, Cadmium (ppm)	20.7	19.7	21.7	20.3	21.1
Ce, Cerium (ppm)	30.1	28.2	32.1	29.5	30.8
Co, Cobalt (ppm)	35.7	34.3	37.2	34.9	36.6
Cr, Chromium (ppm)	27.5	26.0	29.0	26.5	28.4
Cs, Caesium (ppm)	0.82	0.75	0.89	0.79	0.86
Cu, Copper (wt.%)	0.508	0.499	0.517	0.500	0.516
Dy, Dysprosium (ppm)	1.52	1.30	1.74	1.43	1.61
Er, Erbium (ppm)	0.46	0.38	0.54	0.43	0.49
Eu, Europium (ppm)	0.56	0.46	0.66	0.52	0.60
Fe, Iron (wt.%)	10.90	10.58	11.22	10.64	11.15
Ga, Gallium (ppm)	3.49	3.23	3.75	3.38	3.61
Gd, Gadolinium (ppm)	2.52	2.05	2.99	2.40	2.64
Ge, Germanium (ppm)	0.17	0.13	0.21	IND	IND
Hf, Hafnium (ppm)	1.41	1.30	1.53	1.37	1.45
Hg, Mercury (ppm)	1.57	1.47	1.67	1.50	1.64
Ho, Holmium (ppm)	0.21	0.17	0.26	IND	IND
In, Indium (ppm)	0.65	0.62	0.68	0.62	0.67
K, Potassium (wt.%)	0.271	0.259	0.284	0.260	0.282
La, Lanthanum (ppm)	15.0	14.3	15.7	14.7	15.3
Li, Lithium (ppm)	4.42	4.17	4.67	4.25	4.59
Mg, Magnesium (wt.%)	0.250	0.237	0.262	0.242	0.257
Mn, Manganese (wt.%)	0.024	0.023	0.025	0.024	0.025
Mo, Molybdenum (ppm)	29.0	27.6	30.3	28.3	29.6
Na, Sodium (wt.%)	0.065	0.061	0.069	0.063	0.068
Nb, Niobium (ppm)	2.25	1.94	2.55	2.13	2.36
Nd, Neodymium (ppm)	15.2	12.7	17.8	14.9	15.6
Ni, Nickel (ppm)	19.6	18.8	20.4	19.1	20.1
P, Phosphorus (wt.%)	0.018	0.017	0.019	0.017	0.018
Pb, Lead (ppm)	590	567	614	579	601

SI unit equivalents: ppm (parts per million; $1 \times 10^{-6} \equiv \text{mg/kg}$; wt.% (weight per cent) $\equiv \%$ (mass fraction).

Note: intervals may appear asymmetric due to rounding.

IND = indeterminate (due to limited reading resolution of the methods employed. For practical purposes the 95% Expanded Uncertainty can be set between zero and a two times multiple of the upper bound/non-detect limit value).

Table 1 continued.

Constituent	Certified Value	95% Expanded Uncertainty		95% Tolerance Limits	
		Low	High	Low	High
Aqua Regia Digestion continued					
Pr, Praseodymium (ppm)	4.16	3.47	4.85	4.04	4.28
Rb, Rubidium (ppm)	11.3	10.7	12.0	10.9	11.8
S, Sulphur (wt.%)	10.64	10.14	11.15	10.52	10.77
Sb, Antimony (ppm)	36.1	33.2	38.9	34.9	37.3
Sc, Scandium (ppm)	2.46	2.28	2.64	2.35	2.57
Se, Selenium (ppm)	25.4	23.1	27.6	24.2	26.5
Sm, Samarium (ppm)	2.86	2.45	3.28	2.73	3.00
Sn, Tin (ppm)	4.29	3.98	4.59	4.01	4.56
Sr, Strontium (ppm)	18.7	17.7	19.7	18.0	19.4
Tb, Terbium (ppm)	0.30	0.26	0.35	0.28	0.33
Te, Tellurium (ppm)	2.24	2.05	2.44	2.15	2.33
Th, Thorium (ppm)	5.20	4.88	5.53	4.97	5.43
Ti, Titanium (wt.%)	0.036	0.032	0.040	0.035	0.037
Tl, Thallium (ppm)	1.45	1.35	1.54	1.36	1.53
U, Uranium (ppm)	3.45	3.26	3.63	3.34	3.55
V, Vanadium (ppm)	14.2	13.1	15.3	13.6	14.8
W, Tungsten (ppm)	1.65	1.55	1.76	1.59	1.72
Y, Yttrium (ppm)	5.46	5.11	5.82	5.30	5.63
Yb, Ytterbium (ppm)	0.29	0.26	0.31	0.27	0.31
Zn, Zinc (wt.%)	0.485	0.470	0.500	0.476	0.494
Zr, Zirconium (ppm)	51	48	54	50	53

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

Note: intervals may appear asymmetric due to rounding.

Table 2. Indicative Values for OREAS 911.

Constituent	Unit	Value	Constituent	Unit	Value	Constituent	Unit	Value
Infrared Combustion								
C	wt.%	0.143						
Borate / Peroxide Fusion ICP								
Ag	ppm	5.01	B	ppm	34.1	Re	ppm	< 0.1
4-Acid Digestion								
Ba	ppm	144	Hg	ppm	0.75			
Aqua Regia Digestion								
Ba	ppm	26.8	Pt	ppb	< 5	Tm	ppm	0.046
Lu	ppm	0.038	Re	ppm	0.008			
Pd	ppb	< 10	Ta	ppm	0.018			

SI unit equivalents: ppb (parts per billion; 1×10^{-9}) \equiv μ g/kg; ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

Note: the number of significant figures reported is not a reflection of the level of certainty of stated values. They are instead an artefact of ORE's in-house CRM-specific LIMS.

TABLE OF CONTENTS

INTRODUCTION.....	8
INTENDED USE	8
SOURCE MATERIAL.....	9
MINIMUM SAMPLE SIZE.....	9
INSTRUCTIONS FOR HANDLING, STORAGE & CORRECT USE	9
PERIOD OF VALIDITY.....	11
COMMUNITION AND HOMOGENISATION PROCEDURES	11
PHYSICAL PROPERTIES	11
MINERALOGY	12
ANALYTICAL PROGRAM.....	12
PARTICIPATING LABORATORIES	13
STATISTICAL ANALYSIS	14
Certified Values and their uncertainty intervals.....	14
Indicative (uncertified) values	14
Homogeneity Evaluation.....	14
METROLOGICAL TRACEABILITY	16
COMMUTABILITY.....	17
PERFORMANCE GATES	17
PREPARER AND SUPPLIER	26
CERTIFYING OFFICER.....	26
ACCREDITATION.....	26
LEGAL NOTICE.....	26
DOCUMENT HISTORY.....	26
REFERENCES	27

LIST OF TABLES

Table 1. Certified Values, Uncertainty & Tolerance Intervals in OREAS 911.....	2
Table 2. Indicative Values for OREAS 911.....	6
Table 3. Physical properties of OREAS 911.....	11
Table 4. Indicative mineralogy of OREAS 911 by semi-quantitative XRD analysis.....	12
Table 5. Neutron Activation Analysis of Au on 20 x 85 mg subsamples.	15
Table 6. Performance Gates for OREAS 911.....	18

LIST OF FIGURES

Figure 1. Au by Pb Fire Assay in OREAS 911.....	23
Figure 2. Cu by 4-acid digestion in OREAS 911.....	24
Figure 3. Zn by 4-acid digestion in OREAS 911	25

INTRODUCTION

OREAS reference materials are intended to provide a low-cost method of evaluating and improving the quality of analysis of geological samples. To the geologist they provide a means of implementing quality control in analytical data sets generated in exploration from the grass roots level through to prospect evaluation, and in grade control at mining operations. To the analyst they provide an effective means of calibrating analytical equipment, assessing new techniques and routinely monitoring in-house procedures. OREAS reference materials enable users to successfully achieve process control of these tasks because the observed variance from repeated analysis has its origin almost exclusively in the analytical process rather than the reference material itself. In evaluating laboratory performance with this CRM, the section headed 'Instructions for handling and correct use' should be read carefully.

Table 1 presents the certified values together with their associated 95 % expanded uncertainty and tolerance intervals. Table 2 provides indicative values, including major and trace element characterisation, Table 3 lists indicative physical properties, while Table 4 reports indicative mineralogy determined by semi-quantitative XRD analysis, Gold homogeneity, assessed by INAA, is shown in Table 5 and is further demonstrated through a nested ANOVA (see *Homogeneity Evaluation* section). Finally, Table 6 presents the performance gate intervals for all certified values.

Tabulated results of all analytes together with uncorrected means, medians, standard deviations, relative standard deviations and per cent deviation of laboratory means from the corrected mean of means (PDM³) are presented in the detailed certification data for this CRM (**OREAS 911-DataPack.1.0.260401_145125.xlsx**). The certified values and uncertainties in this Certificate are the sole authoritative figures. Any additional significant figures in the DataPack are provided for reference only and do not affect the certified results.

Results are also presented in scatter plots for Au by Pb fire assay and Cu and Zn by 4-acid digestion in Figures 1 to 3 respectively, together with $\pm 3SD$ (magenta) and $\pm 5\%$ (yellow) control lines and certified value (green line). Accepted individual results are coloured blue and individual and dataset outliers are identified in red and violet, respectively.

INTENDED USE

OREAS 911 is intended to cover all activities needed to produce a measurement result. This includes extraction, possible separation steps and the actual measurement process (the signal producing step). OREAS 911 may be used to calibrate the entire procedure by producing a pure substance CRM transformed into a calibration solution.

OREAS 911 is intended for the following uses:

- For the monitoring of laboratory performance in the analysis of analytes reported in Table 1 in geological samples;
- For the verification/ validation of analytical methods for analytes reported in Table 1;
- For the calibration of instruments used in the determination of the concentration of analytes reported in Table 1. When a value provided in this certificate is used to calibrate a measurement process, the uncertainty associated with that value should be appropriately propagated into the user's uncertainty calculation. Users can determine an approximation of the standard uncertainty by calculating one fourth of

the width of the Expanded Uncertainty interval given in this certificate (Expanded Uncertainty intervals are provided in Table 1).

SOURCE MATERIAL

OREAS 911 was prepared from a blend of volcanic-hosted massive sulphide (VMS) ore and barren rhyodacite. The VMS ore was sourced from the Ming Lode, located in Newfoundland and Labrador, Canada. The Ming Lode is characterised by polymetallic sulphide assemblages containing copper, zinc, gold and silver, occurring as semi-massive to massive sulphide zones within volcanic host rocks. Sulphide mineralisation is dominated by pyrite and chalcopyrite hosted within a silica-sericite-altered rhyodacite matrix. The principal sulphide minerals, in approximate order of abundance, are pyrite, chalcopyrite, cubanite, sphalerite, pyrrhotite, arsenopyrite and galena.

MINIMUM SAMPLE SIZE

To relate analytical determinations to the values in this certificate, the minimum mass of sample used should match the typical mass that the laboratories used in the interlaboratory (round robin) certification program. This means that different minimum sample masses should be used depending on the operationally defined methodology as follows:

- Au by lead collection fire assay: ≥ 25 g;
- Au by aqua regia digestion ICP finish: ≥ 15 g;
- Total S by IR combustion furnace/CS analyser: ≥ 0.1 g;
- Borate fusion / Sodium peroxide with ICP-OES and/or MS finish: ≥ 0.2 g;
- 4-acid digestion with ICP-OES and/or MS finish: ≥ 0.25 g;
- Aqua regia digestion with ICP-OES and/or MS finish: ≥ 0.5 g.

INSTRUCTIONS FOR HANDLING, STORAGE & CORRECT USE

Fine powders pose a risk to eyes and lungs and therefore standard precautions including the use of safety glasses and dust masks are advised.

Pre-homogenisation of the CRM prior to subsampling and analysis is not necessary as there is no particle segregation under transport [12].

All certified values contained within this report refer to the concentration levels in the packaged state. There is no need for drying prior to weighing and analysis.

Single-use sachets sealed under nitrogen

OREAS 911 contains a small portion of reactive sulphide material and, as a precaution to mitigate oxidation, is packaged under a nitrogen atmosphere in robust laminated foil pouches. Following analysis, any remaining material should be discarded unless the sachet is promptly resealed under vacuum or nitrogen. It is the user's responsibility to prevent contamination and minimise exposure to the atmosphere.

Authoritative Source of Information

This Certificate of Analysis constitutes the primary and authoritative document for the certified values, associated expanded uncertainties, and their correct use. While the accompanying DataPack provides supporting information, including raw data and uncertainty estimates with additional significant figures, these extended figures are provided solely for transparency, convenience and statistical reference. Users must rely exclusively on the values stated in this Certificate, rounded to an appropriate number of significant figures, for all metrological and analytical purposes. Any discrepancy between values presented in the DataPack and those in this Certificate shall be resolved in favour of the information provided herein.

Notice on Certificate Updates

The version of the Certificate of Analysis (COA) available on the OREAS website is considered the official and most current version. As COAs may be revised following periodic reviews, re-evaluation of data, or the availability of new information, users are strongly advised to refer to the latest online version prior to each use.

It is the user's responsibility to ensure that the most recent and applicable certificate is used to support the traceability, validity, and fitness-for-purpose of the certified reference material (CRM).

Any significant changes to the sections of this certificate will be clearly documented in the revised certificate.

QC monitoring using multiples of the Standard Deviation (SD)

In the application of SD's in monitoring performance it is important to note that not all laboratories function at the same level of proficiency and that different methods in use at a particular laboratory have differing levels of precision. Each laboratory has its own inherent SD (for a specific concentration level and analyte-method pair) based on the analytical process and this SD is not directly related to the round robin program.

The majority of data generated in the round robin program was produced by a selection of world class laboratories. The SD's thus generated are more constrained than those that would be produced across a randomly selected group of laboratories. To produce more generally achievable SD's the 'pooled' SD's provided in this report include interlaboratory bias. This 'one size fits all' approach may require revision at the discretion of the QC manager concerned following careful scrutiny of QC control charts.

The performance gates shown in Table 6 are intended only to be used as a preliminary guide as to what a laboratory may be able to achieve. Over a period of time monitoring your own laboratory's data for this CRM, SD's should be calculated directly from your own laboratory's process. This will enable you to establish more specific performance gates that are fit for purpose for your application as well as the ability to monitor bias. If your long-term trend analysis shows an average value that is within the 95 % expanded uncertainty then generally there is no cause for concern in regard to bias.

For use with the aqua regia digestion method

It is important to note that in the analytical industry there is no standardisation of the aqua regia digestion process. This method is a partial empirical digest and differences in recoveries for various analytes are commonplace. These are caused by variations in the digest conditions and can include the ratio of nitric to hydrochloric acids, acid strength,

temperatures, leach times and secondary digestions. Recoveries for sulphide-hosted base metal sulphides approach total values, however, other analytes, in particular the lithophile elements, show greater sensitivity to method parameters. This can result in lack of consensus in an inter-laboratory certification program for these elements.

The approach applied here is to report certified values in those instances where reasonable agreement exists amongst a majority of participating laboratories. The results of specific laboratories may differ significantly from the certified values, but will, nonetheless, be valid and reproducible in the context of the specifics of the aqua regia method in use. Users of this reference material should, therefore, be mindful of this limitation when applying the certified values in a quality control program.

PERIOD OF VALIDITY

The certification of OREAS 911 remains valid, within the specified measurement uncertainties, until at least July 2040, provided the CRM is handled and stored in accordance with the instructions given below. This certification is nullified if the CRM is any way changed or contaminated.

Store in a clean and cool dry place away from direct sunlight.

Long-term stability will be monitored at appropriate intervals and purchasers notified if any changes are observed. The period of validity may well be indefinite and will be reassessed prior to expiry with the aim of extending the validity if possible.

COMMINUTION AND HOMOGENISATION PROCEDURES

The materials constituting OREAS 911 was prepared in the following manner:

- Drying of ores and barren materials to constant mass at 85 °C;
- Crushing and multi-stage milling of the barren material to >98 % minus 75 microns;
- Crushing and multi-stage milling of the ore to 100 % minus 30 microns;
- Blending the ore and barren material in appropriate proportions to achieve desired grades;
- Homogenisation using OREAS' novel processing technologies;
- Packaging in 60 g units sealed under nitrogen in laminated foil pouches.

PHYSICAL PROPERTIES

OREAS 911 was tested at ORE Research & Exploration Pty Ltd's onsite facility for various physical properties. Table 3 presents these findings that should be used for informational purposes only.

Table 3. Physical properties of OREAS 911.

Bulk Density (kg/m ³)	Moisture (wt.%)	Munsell Notation [‡]	Munsell Color [‡]
674	0.39	N4	Medium Dark Gray

[‡]The Munsell Rock Color Chart helps geologists and archeologists communicate with colour more effectively by cross-referencing ISCC-NBS colour names with unique Munsell alpha-numeric colour notations for rock colour samples.

MINERALOGY

The semi-quantitative XRD results shown in Table 4 below were undertaken by ALS Metallurgy in Balcatta, Western Australia. The results have been normalised to 100 % and represent the relative proportion of crystalline material. Totals greater or less than 100 % are due to rounding errors.

Some amorphous material may be present. 'Clay minerals' appears to be mainly smectite and/or vermiculite. 'Kandite group' appears to be mainly kaolinite. 'K-feldspar and/or rutile' appears to be most likely K-feldspar. A trace of calcite may be present and, if present, is reported under chalcopyrite due to pattern overlap. Minor arsenopyrite and sphalerite is likely present, but this cannot be confirmed due to pattern overlap. A trace of kandite group and/or serpentine may be present.

Table 4. Indicative mineralogy of OREAS 911 by semi-quantitative XRD analysis.

Mineral / Mineral Group	% (mass ratio)
Chalcopyrite	2
Pyrite	20
Magnetite	1
Hematite	< 1
Clay minerals	< 1
Chlorite	1
Annite - biotite - phlogopite	< 1
Muscovite - illite	14
Ca amphibole	2
Plagioclase	23
K-feldspar and/or rutile	7
Quartz	29
Garnet	< 1
Dolomite - ankerite	< 1

ANALYTICAL PROGRAM

Twenty-eight commercial analytical laboratories participated in the program to certify the elements reported in Table 1. The following methods were employed:

- Instrumental neutron activation analysis (INAA) for Au on 20 x 85 mg subsamples to confirm homogeneity (1 laboratory);
- Gold by Pb collection fire assay (25-50g charge weight) with AAS (21 laboratories), ICP-OES or ICP-MS (5 laboratories) finish;
- Gold by 15-50g aqua regia digestion with ICP-MS (10 laboratories) or AAS (6 laboratories) finish;
- Total S by IR combustion furnace (23 laboratories);
- Full ICP-OES and ICP-MS elemental suites by sodium peroxide fusion (up to 18 laboratories depending on the element);
- Full ICP-OES and ICP-MS elemental suites by 4-acid (HNO₃-HF-HClO₄-HCl) digestion (up to 22 laboratories depending on the element);

- Full ICP-OES and ICP-MS elemental suites by aqua regia digestion (up to 22 laboratories depending on the element).

For the round robin program, twelve 2.5 kg test units were collected at predetermined intervals during the bagging stage, immediately after homogenisation. The samples received by each laboratory were obtained by taking a 160 g sample from six different 2.5 kg test units to maximise representation (i.e., from either the odd or even sampling (lot) intervals).

The 20 individual INAA results upon which much of the homogeneity evaluation is based, included paired 10 g samples taken from 10 different sampling units. This format enabled a nested ANOVA treatment of the INAA results to evaluate homogeneity (see 'Homogeneity Evaluation' section below).

PARTICIPATING LABORATORIES

1. Actlabs, Ancaster, Ontario, Canada
2. AGAT Laboratories, Thunder Bay, Ontario, Canada
3. ALS, Brisbane, QLD, Australia
4. ALS, Lima, Peru
5. ALS, Loughrea, Galway, Ireland
6. ALS, Malaga, WA, Australia
7. ALS, Vancouver, BC, Canada
8. American Assay Laboratories, Sparks, Nevada, USA
9. ANSTO, Lucas Heights, NSW, Australia
10. Bureau Veritas Commodities Canada Ltd, Vancouver, BC, Canada
11. Gekko Assay Labs, Ballarat, VIC, Australia
12. Inspectorate (BV), Lima, Peru
13. Intertek, Cupang, Muntinlupa, Philippines
14. Intertek, Perth, WA, Australia
15. Intertek, Townsville, QLD, Australia
16. Intertek Genalysis, Adelaide, SA, Australia
17. Intertek Minerals Ltd, Tarkwa, Western Region, Ghana
18. Lucid Laboratories Private Limited, Hyderabad, Telangana, India
19. On Site Laboratory Services, Bendigo, VIC, Australia
20. PT Geoservices Ltd, Cikarang, Jakarta Raya, Indonesia
21. PT Indo Mineral Research, Bungursari, West Java, Indonesia
22. PT Intertek Utama Services, Jakarta Timur, DKI Jakarta, Indonesia
23. SGS Canada Inc., Vancouver, BC, Canada
24. SGS Geosol Laboratorios Ltda, Vespasiano, Minas Gerais, Brazil
25. SGS Tarkwa, Tarkwa, Western Region, Ghana
26. Shiva Analyticals Ltd, Bangalore North, Karnataka, India
27. Skyline Assayers & Laboratories, Tucson, Arizona, USA
28. Stewart Assay & Environmental Laboratories LLC, Kara-Balta, Chüy, Kyrgyzstan

Please note: To maintain anonymity of participating laboratories, the alphabetical list above does not correspond to the Lab ID numbers shown in the scatter plots below.

STATISTICAL ANALYSIS

Certified Values and their uncertainty intervals (Table 1) have been determined for each analyte following removal of individual, laboratory dataset (batch) and 3SD outliers (single iteration). Outlier evaluation was conducted in accordance with ISO 17034:2017 and ISO 33405:2024. While formal statistical tests were applied, professional statistical judgment was also exercised in determining the validity of potential outliers. Assessment of systematic bias and performance using independent control materials (CRMs) was incorporated to ensure compliance with the referenced standards and to establish metrological traceability of the certified values.

95% Expanded Uncertainty provides a 95 % probability that the true value of the analyte under consideration lies between the upper and lower limits and is calculated according to the method outlined in [6] and [15]. All known or suspected sources of bias have been investigated or taken into account.

Indicative (uncertified) values (Table 2) are present where the number of laboratories reporting a particular analyte is insufficient (< 5) to support certification or where interlaboratory consensus is poor. This data is intended for 'informational purposes' only.

Standard Deviation intervals (see Table 6, 'Performance Gates') provide an indication of a level of performance that might reasonably be expected from a laboratory being monitored by this CRM in a QA/QC program. They take into account errors attributable to measurement uncertainty and CRM variability. For an effective CRM the contribution of the latter should be negligible in comparison to measurement errors. The Standard Deviation values include all sources of measurement uncertainty: between-lab variance, within-run variance (precision errors) and CRM variability.

The SD for each analyte's certified value is calculated from the same filtered data set used to determine the certified value, i.e., after removal of all individual, lab dataset (batch) and 3SD outliers (single iteration). These outliers can only be removed after the absolute homogeneity of the CRM has been independently established, i.e., the outliers must be confidently deemed to be analytical rather than arising from inhomogeneity of the CRM. ***The standard deviation is then calculated for each analyte from the pooled accepted analyses generated from the certification program.***

Homogeneity Evaluation

For analytes other than gold, the tolerance limits (ISO 16269:2014) shown in Table 1 were determined using an analysis of precision errors method and are considered a conservative estimate of true homogeneity. The meaning of tolerance limits may be illustrated for Cu by 4-acid digestion, where 99 % of the time ($1-\alpha=0.99$) at least 95 % of subsamples ($\rho=0.95$) will have concentrations lying between 0.488 and 0.504 wt.%. Put more precisely, this means that if the same number of subsamples were taken and analysed in the same manner repeatedly, 99 % of the tolerance intervals so constructed would cover at least 95 % of the total population, and 1 % of the tolerance intervals would cover less than 95 % of the total population. ***Please note that tolerance limits pertain to the homogeneity of the CRM only and should not be used as control limits for laboratory performance.***

The homogeneity of gold has been determined by INAA at ANSTO using the reduced analytical subsample method which utilises the known relationship between standard deviation and analytical subsample weight (Ingamells and Switzer, 1973 [2]). In this approach the sample aliquot is substantially reduced to a point where most of the variability in replicate assays should be due to inhomogeneity of the reference material and

measurement error becomes negligible. Table 5 below shows the gold INAA data determined on 20 x 85 mg subsamples of OREAS 911. An equivalent scaled version of the results is also provided to demonstrate an appreciation of what this data means if 30 g fire assays were undertaken without the normal measurement error associated with this methodology. In this instance, the 1RSD of 0.12 % calculated for a 30 g fire assay sample (2.31 % at 85 mg weights) confirms the high level of gold homogeneity in OREAS 911.

Table 5. Neutron Activation Analysis of Au (in ppm) on 20 x 85 mg subsamples and showing the equivalent results scaled to a 30 g sample mass typical of fire assay determination.

Replicate No	Au 85 mg actual	Au 30 g equivalent*
1	0.771	0.791
2	0.770	0.791
3	0.812	0.793
4	0.796	0.792
5	0.804	0.792
6	0.769	0.791
7	0.803	0.792
8	0.764	0.790
9	0.767	0.791
10	0.788	0.792
11	0.822	0.793
12	0.793	0.792
13	0.802	0.792
14	0.814	0.793
15	0.803	0.792
16	0.816	0.793
17	0.774	0.791
18	0.799	0.792
19	0.777	0.791
20	0.794	0.792
Mean	0.792	0.792
Median	0.795	0.792
Std Dev.	0.018	0.001
Rel.Std.Dev.	2.31%	0.12%

*Results calculated for a 30 g equivalent sample mass using the formula: $x^{30g Eq} = \frac{(x^{INAA} - \bar{X}) \times RSD@30g}{RSD@85mg} + \bar{X}$

where $x^{30g Eq}$ = equivalent result calculated for a 30 g sample mass

(x^{INAA}) = raw INAA result at 85 mg

\bar{X} = mean of 85 mg INAA results

The homogeneity of OREAS 911 has also been evaluated in an Analysis of Variance (**ANOVA**) of the INAA data. The 20 samples were comprised of paired samples from each of 10 sampling lot intervals (representative of the prepared batch) and were randomised prior to assigning sample numbers. The duplicate samples enabled an ANOVA by comparison of within- and between-unit variances across the 10 pairs. The purpose of the ANOVA is to test that no statistically significant difference exists in the variance between units to that of the variance within units. This allows an assessment of homogeneity across the entire prepared batch of OREAS 911. The test was performed using the following parameters:

- Gold INAA – 20 results (1 laboratory providing duplicate analyses on 10 samples where each sample can be viewed as a ‘unit’);

- Null Hypothesis, H_0 : Between-unit variance is no greater than within-unit variance (reject H_0 if p -value < 0.05);
- Alternative Hypothesis, H_1 : Between-unit variance is greater than within-unit variance.

The data were not filtered for outliers before p -value calculation, which yielded 0.25—statistically insignificant, so the Null Hypothesis is accepted. ANOVA does not measure absolute homogeneity; it evaluates whether analytes are similarly distributed across the packaging run and whether variance between subsamples from the same unit differs from that between separate units. A reference material may show poor absolute homogeneity yet still meet a relative homogeneity (ANOVA) criterion if within-unit heterogeneity is substantial and consistent. Based on ANOVA and interlaboratory certification results, OREAS 911 is fit-for-purpose as a certified reference material (see ‘Intended Use’ above).

METROLOGICAL TRACEABILITY

The interlaboratory results that underpin the certified values are metrologically traceable to the international measurement scale (SI) of mass (either as a % mass fraction or as milligrams per kilogram (mg/kg)) [14]. In line with popular use, all data within tables in this certificate are expressed as the mass fraction in either weight percent (wt.%) or parts per million (ppm).

The analytical samples sent to participating laboratories were selected in a manner to be representative of the entire prepared batch of CRM. This representativeness was maintained in each submitted laboratory sample batch and ensures the user that the data is traceable from sample selection through to the analytical results. The systematic sampling method was chosen due to the low risk of overlooking repetitive effects or trends in the batch due to the way the CRM was processed. In line with ISO 17025 [8], each analytical data set received from the participating laboratories has been validated by its assayer through the inclusion of internal reference materials and QC checks during and post analysis.

Participating laboratories were selected based on demonstrated analytical competence, including prior performance in interlaboratory comparison programs conducted by ORE Pty Ltd, with consideration given to their expertise in relevant analytical methods, measurands, and sample matrices. For the measurands reported in this certificate (Table 1), data were sourced from laboratories accredited to ISO/IEC 17025. Where formal accreditation was not held for specific operationally defined measurands, metrological traceability was verified through the use of well-characterised, independently certified reference materials (CRMs) included as control samples in the round robin study.

In accordance with ISO 33405:2024-05 [5], clause 9.2.5, and ISO 17034:2016 [9], clause 7.12.4 b), the use of such control samples provides an acceptable means of demonstrating traceability in the absence of formal accreditation. In this certification program, traceability was further supported by the agreement of measured values for control samples with their known certified values, thereby offering additional confidence in the calibration and validity of measurement results across participating laboratories.

Operationally Defined Measurands

In accordance with ISO 33405:2024-05, Clause 9.2.4, measurands (analytes) may be certified as operationally defined. For these measurands, traceability to the SI may not be achievable because the analytical procedure involves sample transformations (e.g.,

leaching or extraction). While instrument calibration can be traceable to appropriate units, the transformation steps themselves are not directly traceable and can only be evaluated through reference comparisons or harmonized procedures.

Accordingly, characterisation of these measurands has been based on the concordance of results obtained from multiple laboratories using a common, well-defined procedure. This approach ensures fitness-for-purpose and fulfils the requirements for metrological traceability as specified in ISO 17034 and ISO 33405 for operationally defined measurands.

COMMUTABILITY

The certified values reported herein are derived from measurements performed using analytical methods involving sample pre-treatment steps, such as fusion or acid digestion. These processes convert the sample matrix into a chemically simplified and stable form, facilitating calibration traceable to primary standards via solution-based calibration protocols. Due to the established robustness and effectiveness of these pre-treatment methods, issues related to commutability are not expected to impact the suitability of this Certified Reference Material (CRM) for its intended use.

OREAS CRMs are prepared from natural ore materials, ensuring the presence of matrix and mineralogical characteristics representative of typical exploration, mine and process samples. Consistent with ISO 17034:2016 and ISO Guide 30, users are advised to select CRMs with matrix and mineralisation styles closely matching those of their routine samples to minimize matrix effects and enhance analytical comparability. Detailed descriptions of the CRM's source material and mineralogical characteristics are provided in the 'Source Material' section to guide appropriate CRM selection.

PERFORMANCE GATES

Table 6 below shows intervals calculated for two and three standard deviations. As a guide these intervals may be regarded as warning or rejection for multiple 2SD outliers, or rejection for individual 3SD outliers in QC monitoring, although their precise application should be at the discretion of the QC manager concerned (also see 'Intended Use' section below). Westgard Rules extend the basics of single-rule QC monitoring using multi-rules (for more information visit www.westgard.com/mltirule.htm). A second method utilises a 5 % window calculated directly from the certified value.

Standard deviation is also shown in relative percent for one, two and three relative standard deviations (1RSD, 2RSD and 3RSD) to facilitate an appreciation of the magnitude of these numbers and a comparison with the 5 % window. Caution should be exercised when concentration levels approach lower limits of detection of the analytical methods employed as performance gates calculated from standard deviations tend to be excessively wide whereas those determined by the 5 % method are too narrow. One approach used at commercial laboratories is to set the acceptance criteria at twice the detection level (DL) ± 10 %.

i.e., Certified Value ± 10 % $\pm 2DL$ [1].

Table 6. Performance Gates for OREAS 911.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5 % window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
Pb Fire Assay											
Au, ppm	0.762	0.038	0.686	0.838	0.648	0.876	4.99%	9.98%	14.97%	0.724	0.800
Aqua Regia Digestion (sample weights 15-50g)											
Au, ppm	0.750	0.038	0.675	0.825	0.637	0.863	5.00%	10.01%	15.01%	0.713	0.788
Infrared Combustion											
S, wt. %	11.00	0.234	10.53	11.46	10.30	11.70	2.12%	4.25%	6.37%	10.45	11.55
Borate / Peroxide Fusion ICP											
Al, wt. %	6.19	0.136	5.92	6.46	5.78	6.60	2.19%	4.38%	6.57%	5.88	6.50
As, ppm	477	11	454	500	443	511	2.37%	4.75%	7.12%	453	501
Ba, ppm	1717	85	1548	1887	1463	1972	4.94%	9.88%	14.83%	1632	1803
Be, ppm	1.90	0.22	1.46	2.35	1.23	2.58	11.77%	23.53%	35.30%	1.81	2.00
Bi, ppm	2.31	0.202	1.91	2.71	1.70	2.91	8.73%	17.46%	26.19%	2.19	2.42
Ca, wt. %	1.27	0.057	1.16	1.39	1.10	1.45	4.50%	8.99%	13.49%	1.21	1.34
Cd, ppm	19.7	1.41	16.8	22.5	15.4	23.9	7.19%	14.38%	21.58%	18.7	20.7
Ce, ppm	56	2.6	51	61	48	64	4.67%	9.34%	14.01%	53	59
Co, ppm	35.8	2.15	31.5	40.1	29.4	42.3	5.99%	11.98%	17.97%	34.0	37.6
Cr, ppm	57	8	40	74	32	82	14.84%	29.69%	44.53%	54	60
Cs, ppm	3.76	0.309	3.14	4.38	2.83	4.69	8.22%	16.45%	24.67%	3.57	3.95
Cu, wt. %	0.506	0.021	0.465	0.548	0.444	0.569	4.11%	8.22%	12.33%	0.481	0.532
Dy, ppm	2.48	0.171	2.14	2.82	1.97	2.99	6.89%	13.78%	20.66%	2.36	2.61
Er, ppm	0.84	0.062	0.71	0.96	0.65	1.02	7.37%	14.74%	22.11%	0.80	0.88
Eu, ppm	0.91	0.10	0.71	1.11	0.61	1.21	11.03%	22.06%	33.08%	0.87	0.96
Fe, wt. %	11.64	0.258	11.13	12.16	10.87	12.42	2.21%	4.43%	6.64%	11.06	12.22
Ga, ppm	18.3	1.54	15.2	21.4	13.7	22.9	8.39%	16.79%	25.18%	17.4	19.2
Gd, ppm	3.80	0.247	3.31	4.29	3.06	4.54	6.51%	13.01%	19.52%	3.61	3.99
Ge, ppm	2.71	0.37	1.98	3.44	1.61	3.81	13.50%	27.00%	40.50%	2.57	2.85
Hf, ppm	4.63	0.364	3.90	5.35	3.53	5.72	7.87%	15.74%	23.61%	4.39	4.86
Ho, ppm	0.38	0.026	0.33	0.43	0.30	0.45	6.76%	13.52%	20.29%	0.36	0.40
In, ppm	0.65	0.055	0.54	0.76	0.48	0.81	8.51%	17.01%	25.52%	0.62	0.68
K, wt. %	2.36	0.095	2.17	2.55	2.07	2.64	4.04%	8.08%	12.12%	2.24	2.48
La, ppm	27.9	1.49	24.9	30.9	23.4	32.4	5.34%	10.67%	16.01%	26.5	29.3
Li, ppm	16.3	2.9	10.4	22.2	7.5	25.1	17.95%	35.91%	53.86%	15.5	17.1
Lu, ppm	0.076	0.012	0.052	0.099	0.041	0.111	15.46%	30.93%	46.39%	0.072	0.079
Mg, wt. %	0.400	0.017	0.365	0.434	0.348	0.452	4.34%	8.68%	13.02%	0.380	0.420
Mn, wt. %	0.031	0.001	0.029	0.033	0.028	0.034	3.02%	6.03%	9.05%	0.030	0.033
Mo, ppm	29.9	2.19	25.5	34.3	23.3	36.5	7.32%	14.65%	21.97%	28.4	31.4
Nb, ppm	11.7	0.65	10.4	13.0	9.7	13.6	5.59%	11.18%	16.77%	11.1	12.2
Nd, ppm	24.1	0.80	22.5	25.7	21.7	26.5	3.31%	6.63%	9.94%	22.9	25.3
Ni, ppm	25.1	5.2	14.7	35.5	9.4	40.7	20.78%	41.57%	62.35%	23.8	26.3
P, wt. %	0.023	0.004	0.014	0.031	0.010	0.035	18.53%	37.07%	55.60%	0.022	0.024
Pb, ppm	614	35	544	683	510	718	5.65%	11.29%	16.94%	583	644
Pr, ppm	6.50	0.303	5.89	7.11	5.59	7.41	4.66%	9.33%	13.99%	6.18	6.83
Rb, ppm	94	2.5	89	99	86	101	2.65%	5.29%	7.94%	89	98
S, wt. %	11.03	0.251	10.53	11.53	10.28	11.78	2.27%	4.54%	6.82%	10.48	11.58

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt.% (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding; IND = indeterminate.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Table 6 continued.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5 % window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
Borate / Peroxide Fusion ICP continued											
Sb, ppm	49.1	2.27	44.6	53.6	42.3	55.9	4.62%	9.23%	13.85%	46.6	51.5
Sc, ppm	< 10	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Se, ppm	25.7	4.8	16.1	35.3	11.3	40.1	18.64%	37.28%	55.92%	24.4	27.0
SiO ₂ , wt. %	54.71	1.596	51.52	57.91	49.92	59.50	2.92%	5.84%	8.75%	51.98	57.45
Sm, ppm	4.66	0.231	4.20	5.12	3.97	5.36	4.95%	9.91%	14.86%	4.43	4.90
Sn, ppm	8.31	0.713	6.88	9.74	6.17	10.45	8.58%	17.16%	25.74%	7.89	8.73
Sr, ppm	129	7	114	143	107	151	5.66%	11.31%	16.97%	122	135
Ta, ppm	0.93	0.16	0.61	1.25	0.45	1.41	17.08%	34.15%	51.23%	0.88	0.98
Tb, ppm	0.51	0.036	0.44	0.59	0.41	0.62	6.91%	13.81%	20.72%	0.49	0.54
Te, ppm	2.20	0.44	1.31	3.09	0.87	3.53	20.16%	40.33%	60.49%	2.09	2.31
Th, ppm	8.79	0.356	8.08	9.51	7.73	9.86	4.04%	8.09%	12.13%	8.35	9.23
Ti, wt. %	0.135	0.006	0.124	0.147	0.118	0.153	4.33%	8.65%	12.98%	0.129	0.142
Tl, ppm	5.00	0.271	4.46	5.54	4.19	5.82	5.43%	10.85%	16.28%	4.75	5.25
Tm, ppm	0.098	0.010	0.077	0.119	0.066	0.129	10.71%	21.43%	32.14%	0.093	0.103
U, ppm	5.30	0.174	4.96	5.65	4.78	5.83	3.28%	6.57%	9.85%	5.04	5.57
V, ppm	43.8	2.36	39.1	48.6	36.7	50.9	5.39%	10.78%	16.17%	41.6	46.0
W, ppm	3.42	0.61	2.21	4.63	1.60	5.24	17.73%	35.47%	53.20%	3.25	3.59
Y, ppm	11.3	0.47	10.3	12.2	9.9	12.7	4.14%	8.28%	12.43%	10.7	11.8
Yb, ppm	0.60	0.08	0.44	0.75	0.37	0.83	12.90%	25.81%	38.71%	0.57	0.63
Zn, wt. %	0.497	0.024	0.449	0.546	0.424	0.570	4.90%	9.80%	14.69%	0.472	0.522
Zr, ppm	179	16	147	212	131	228	8.95%	17.90%	26.85%	170	188
4-Acid Digestion											
Ag, ppm	4.70	0.216	4.27	5.13	4.05	5.35	4.60%	9.20%	13.80%	4.46	4.93
Al, wt. %	6.03	0.214	5.60	6.46	5.39	6.67	3.54%	7.09%	10.63%	5.73	6.33
As, ppm	463	16	430	495	414	512	3.53%	7.06%	10.59%	439	486
Be, ppm	1.87	0.075	1.72	2.02	1.64	2.09	4.03%	8.06%	12.09%	1.77	1.96
Bi, ppm	2.41	0.113	2.19	2.64	2.08	2.75	4.66%	9.33%	13.99%	2.29	2.54
Ca, wt. %	1.26	0.041	1.17	1.34	1.13	1.38	3.24%	6.48%	9.72%	1.19	1.32
Cd, ppm	20.7	0.88	18.9	22.4	18.0	23.3	4.24%	8.49%	12.73%	19.6	21.7
Ce, ppm	51	2.7	45	56	43	59	5.36%	10.72%	16.07%	48	53
Co, ppm	36.6	0.91	34.8	38.5	33.9	39.4	2.49%	4.99%	7.48%	34.8	38.5
Cr, ppm	46.8	3.76	39.3	54.3	35.5	58.1	8.04%	16.07%	24.11%	44.5	49.2
Cs, ppm	3.70	0.219	3.26	4.14	3.04	4.36	5.92%	11.84%	17.76%	3.52	3.89
Cu, wt. %	0.496	0.015	0.466	0.526	0.452	0.540	2.99%	5.97%	8.96%	0.471	0.521
Dy, ppm	2.41	0.177	2.06	2.77	1.88	2.94	7.34%	14.68%	22.01%	2.29	2.53
Er, ppm	0.80	0.055	0.69	0.91	0.64	0.97	6.82%	13.63%	20.45%	0.76	0.84
Eu, ppm	0.87	0.025	0.82	0.92	0.80	0.95	2.89%	5.78%	8.67%	0.83	0.91
Fe, wt. %	11.42	0.297	10.83	12.02	10.53	12.31	2.60%	5.20%	7.79%	10.85	11.99
Ga, ppm	18.5	0.73	17.0	19.9	16.3	20.6	3.93%	7.86%	11.80%	17.5	19.4
Gd, ppm	3.75	0.224	3.30	4.20	3.08	4.42	5.98%	11.95%	17.93%	3.56	3.94
Ge, ppm	0.25	0.07	0.11	0.39	0.04	0.46	28.33%	56.65%	84.98%	0.24	0.26
Hf, ppm	4.55	0.226	4.10	5.00	3.87	5.23	4.97%	9.95%	14.92%	4.32	4.78
Ho, ppm	0.35	0.028	0.30	0.41	0.27	0.44	7.93%	15.85%	23.78%	0.34	0.37

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt. % (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Table 6 continued.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5 % window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
4-Acid Digestion continued											
In, ppm	0.67	0.029	0.61	0.72	0.58	0.75	4.42%	8.84%	13.26%	0.63	0.70
K, wt. %	2.31	0.077	2.16	2.47	2.08	2.55	3.33%	6.66%	9.99%	2.20	2.43
La, ppm	23.4	1.86	19.7	27.1	17.8	29.0	7.93%	15.86%	23.78%	22.2	24.6
Li, ppm	15.0	0.96	13.1	17.0	12.2	17.9	6.38%	12.76%	19.14%	14.3	15.8
Lu, ppm	0.077	0.007	0.063	0.092	0.056	0.099	9.26%	18.51%	27.77%	0.074	0.081
Mg, wt. %	0.378	0.015	0.348	0.407	0.333	0.422	3.95%	7.90%	11.85%	0.359	0.396
Mn, wt. %	0.031	0.001	0.029	0.032	0.028	0.033	2.71%	5.42%	8.13%	0.029	0.032
Mo, ppm	30.0	0.97	28.1	32.0	27.1	33.0	3.23%	6.46%	9.69%	28.5	31.5
Na, wt. %	1.72	0.047	1.62	1.81	1.58	1.86	2.72%	5.43%	8.15%	1.63	1.80
Nb, ppm	11.5	0.59	10.3	12.6	9.7	13.2	5.12%	10.25%	15.37%	10.9	12.0
Nd, ppm	23.3	1.30	20.7	25.9	19.4	27.2	5.57%	11.14%	16.71%	22.1	24.5
Ni, ppm	20.5	1.02	18.4	22.5	17.4	23.5	4.98%	9.96%	14.95%	19.4	21.5
P, wt. %	0.020	0.001	0.019	0.022	0.018	0.023	4.13%	8.25%	12.38%	0.019	0.021
Pb, ppm	601	25	551	650	526	675	4.12%	8.25%	12.37%	570	631
Pr, ppm	6.09	0.400	5.29	6.89	4.89	7.29	6.56%	13.13%	19.69%	5.79	6.40
Rb, ppm	91	4.7	82	100	77	105	5.20%	10.40%	15.59%	86	96
Re, ppm	0.008	0.001	0.005	0.011	0.004	0.012	15.70%	31.39%	47.09%	0.008	0.008
S, wt. %	10.48	0.653	9.17	11.79	8.52	12.44	6.23%	12.47%	18.70%	9.95	11.00
Sb, ppm	47.3	2.96	41.4	53.2	38.4	56.2	6.26%	12.51%	18.77%	44.9	49.7
Sc, ppm	8.21	0.416	7.38	9.04	6.96	9.46	5.07%	10.13%	15.20%	7.80	8.62
Se, ppm	25.3	2.8	19.8	30.9	17.1	33.6	10.89%	21.78%	32.67%	24.1	26.6
Sm, ppm	4.50	0.299	3.90	5.09	3.60	5.39	6.65%	13.30%	19.95%	4.27	4.72
Sn, ppm	7.67	0.408	6.85	8.49	6.44	8.89	5.33%	10.65%	15.98%	7.29	8.05
Sr, ppm	118	6	105	130	99	137	5.39%	10.78%	16.17%	112	124
Ta, ppm	0.83	0.039	0.76	0.91	0.72	0.95	4.64%	9.28%	13.92%	0.79	0.88
Tb, ppm	0.51	0.035	0.44	0.59	0.41	0.62	6.89%	13.77%	20.66%	0.49	0.54
Te, ppm	2.19	0.199	1.80	2.59	1.60	2.79	9.08%	18.17%	27.25%	2.08	2.30
Th, ppm	7.79	0.81	6.17	9.41	5.36	10.22	10.40%	20.81%	31.21%	7.40	8.18
Ti, wt. %	0.112	0.006	0.101	0.123	0.095	0.128	4.97%	9.94%	14.90%	0.106	0.117
Tl, ppm	4.96	0.238	4.49	5.44	4.25	5.68	4.80%	9.61%	14.41%	4.71	5.21
Tm, ppm	0.089	0.017	0.055	0.122	0.039	0.139	18.82%	37.63%	56.45%	0.084	0.093
U, ppm	5.16	0.287	4.59	5.74	4.30	6.02	5.55%	11.10%	16.65%	4.91	5.42
V, ppm	43.9	2.22	39.5	48.4	37.2	50.6	5.07%	10.13%	15.20%	41.7	46.1
W, ppm	3.19	0.169	2.85	3.53	2.69	3.70	5.30%	10.61%	15.91%	3.03	3.35
Y, ppm	11.1	0.43	10.2	11.9	9.8	12.4	3.88%	7.76%	11.64%	10.5	11.6
Yb, ppm	0.57	0.040	0.49	0.65	0.45	0.69	7.06%	14.11%	21.17%	0.54	0.60
Zn, wt. %	0.494	0.016	0.461	0.527	0.445	0.543	3.32%	6.64%	9.96%	0.469	0.519
Zr, ppm	170	6	158	182	152	188	3.61%	7.21%	10.82%	162	179
Aqua Regia Digestion											
Ag, ppm	4.80	0.253	4.30	5.31	4.04	5.56	5.27%	10.53%	15.80%	4.56	5.04
Al, wt. %	0.753	0.034	0.685	0.822	0.650	0.856	4.55%	9.11%	13.66%	0.716	0.791
As, ppm	459	13	432	485	419	498	2.88%	5.76%	8.64%	436	482
B, ppm	< 10	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt. % (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Table 6 continued.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5 % window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
Aqua Regia Digestion continued											
Be, ppm	0.29	0.010	0.27	0.31	0.26	0.32	3.43%	6.86%	10.29%	0.28	0.30
Bi, ppm	2.37	0.103	2.16	2.58	2.06	2.68	4.37%	8.74%	13.10%	2.25	2.49
Ca, wt. %	0.714	0.037	0.640	0.789	0.602	0.826	5.23%	10.46%	15.69%	0.679	0.750
Cd, ppm	20.7	1.03	18.6	22.8	17.6	23.8	4.98%	9.96%	14.94%	19.7	21.7
Ce, ppm	30.1	1.61	26.9	33.4	25.3	35.0	5.36%	10.72%	16.08%	28.6	31.6
Co, ppm	35.7	1.16	33.4	38.0	32.3	39.2	3.24%	6.47%	9.71%	33.9	37.5
Cr, ppm	27.5	2.01	23.4	31.5	21.4	33.5	7.33%	14.66%	21.99%	26.1	28.8
Cs, ppm	0.82	0.09	0.64	1.00	0.55	1.09	10.99%	21.98%	32.98%	0.78	0.86
Cu, wt. %	0.508	0.010	0.488	0.527	0.478	0.537	1.93%	3.86%	5.78%	0.482	0.533
Dy, ppm	1.52	0.18	1.16	1.88	0.98	2.06	11.90%	23.79%	35.69%	1.44	1.59
Er, ppm	0.46	0.06	0.35	0.58	0.29	0.63	12.52%	25.05%	37.57%	0.44	0.48
Eu, ppm	0.56	0.07	0.42	0.69	0.35	0.76	12.17%	24.34%	36.50%	0.53	0.59
Fe, wt. %	10.90	0.361	10.18	11.62	9.82	11.98	3.31%	6.62%	9.93%	10.35	11.44
Ga, ppm	3.49	0.329	2.83	4.15	2.50	4.48	9.43%	18.86%	28.28%	3.32	3.67
Gd, ppm	2.52	0.40	1.71	3.33	1.31	3.73	16.03%	32.05%	48.08%	2.39	2.65
Ge, ppm	0.17	0.03	0.11	0.22	0.09	0.25	16.48%	32.95%	49.43%	0.16	0.18
Hf, ppm	1.41	0.15	1.12	1.70	0.98	1.85	10.29%	20.57%	30.86%	1.34	1.48
Hg, ppm	1.57	0.097	1.38	1.76	1.28	1.86	6.18%	12.36%	18.54%	1.49	1.65
Ho, ppm	0.21	0.04	0.14	0.29	0.10	0.32	17.72%	35.43%	53.15%	0.20	0.22
In, ppm	0.65	0.023	0.60	0.69	0.58	0.72	3.59%	7.18%	10.77%	0.61	0.68
K, wt. %	0.271	0.014	0.243	0.300	0.229	0.314	5.24%	10.47%	15.71%	0.258	0.285
La, ppm	15.0	0.74	13.5	16.5	12.8	17.2	4.93%	9.85%	14.78%	14.2	15.7
Li, ppm	4.42	0.336	3.75	5.09	3.41	5.43	7.61%	15.22%	22.83%	4.20	4.64
Mg, wt. %	0.250	0.015	0.220	0.280	0.205	0.295	6.05%	12.09%	18.14%	0.237	0.262
Mn, wt. %	0.024	0.001	0.022	0.026	0.021	0.028	4.66%	9.32%	13.99%	0.023	0.025
Mo, ppm	29.0	1.44	26.1	31.9	24.6	33.3	4.98%	9.95%	14.93%	27.5	30.4
Na, wt. %	0.065	0.007	0.051	0.079	0.044	0.086	10.82%	21.63%	32.45%	0.062	0.069
Nb, ppm	2.25	0.39	1.47	3.03	1.08	3.41	17.33%	34.66%	51.99%	2.13	2.36
Nd, ppm	15.2	2.1	11.0	19.5	8.9	21.6	13.80%	27.60%	41.40%	14.5	16.0
Ni, ppm	19.6	0.61	18.4	20.8	17.8	21.4	3.12%	6.25%	9.37%	18.6	20.6
P, wt. %	0.018	0.001	0.016	0.019	0.015	0.020	4.48%	8.97%	13.45%	0.017	0.019
Pb, ppm	590	25	541	639	517	664	4.15%	8.30%	12.45%	561	620
Pr, ppm	4.16	0.58	3.01	5.32	2.43	5.89	13.87%	27.73%	41.60%	3.95	4.37
Rb, ppm	11.3	0.67	10.0	12.7	9.3	13.3	5.90%	11.81%	17.71%	10.8	11.9
S, wt. %	10.64	0.591	9.46	11.83	8.87	12.42	5.55%	11.10%	16.64%	10.11	11.18
Sb, ppm	36.1	4.6	26.8	45.3	22.1	50.0	12.87%	25.74%	38.61%	34.3	37.9
Sc, ppm	2.46	0.142	2.17	2.74	2.03	2.89	5.79%	11.58%	17.36%	2.34	2.58
Se, ppm	25.4	3.6	18.1	32.6	14.5	36.2	14.28%	28.55%	42.83%	24.1	26.6
Sm, ppm	2.86	0.34	2.18	3.54	1.84	3.88	11.88%	23.76%	35.64%	2.72	3.01
Sn, ppm	4.29	0.296	3.69	4.88	3.40	5.17	6.90%	13.81%	20.71%	4.07	4.50
Sr, ppm	18.7	1.03	16.7	20.8	15.6	21.8	5.49%	10.99%	16.48%	17.8	19.7
Tb, ppm	0.30	0.030	0.24	0.36	0.21	0.39	9.80%	19.59%	29.39%	0.29	0.32
Te, ppm	2.24	0.216	1.81	2.67	1.59	2.89	9.65%	19.31%	28.96%	2.13	2.35

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt. % (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD and 3SD windows.

Table 6 continued.

Constituent	Certified Value	Absolute Standard Deviations					Relative Standard Deviations			5 % window	
		1SD	2SD Low	2SD High	3SD Low	3SD High	1RSD	2RSD	3RSD	Low	High
Aqua Regia Digestion continued											
Th, ppm	5.20	0.299	4.60	5.80	4.31	6.10	5.75%	11.51%	17.26%	4.94	5.46
Ti, wt. %	0.036	0.008	0.021	0.051	0.014	0.059	20.74%	41.49%	62.23%	0.034	0.038
Tl, ppm	1.45	0.116	1.21	1.68	1.10	1.80	8.04%	16.08%	24.13%	1.37	1.52
U, ppm	3.45	0.198	3.05	3.84	2.85	4.04	5.75%	11.50%	17.25%	3.28	3.62
V, ppm	14.2	1.6	11.1	17.3	9.5	18.9	10.97%	21.94%	32.90%	13.5	14.9
W, ppm	1.65	0.089	1.48	1.83	1.39	1.92	5.39%	10.78%	16.18%	1.57	1.74
Y, ppm	5.46	0.476	4.51	6.41	4.04	6.89	8.70%	17.41%	26.11%	5.19	5.74
Yb, ppm	0.29	0.018	0.25	0.33	0.23	0.34	6.36%	12.72%	19.08%	0.27	0.30
Zn, wt. %	0.485	0.017	0.451	0.519	0.434	0.536	3.51%	7.02%	10.52%	0.461	0.509
Zr, ppm	51	3.6	44	58	40	62	6.98%	13.96%	20.93%	49	54

SI unit equivalents: ppm (parts per million; 1×10^{-6}) \equiv mg/kg; wt. % (weight per cent) \equiv % (mass fraction).

Note 1: intervals may appear asymmetric due to rounding.

Note 2: the number of decimal places quoted does not imply accuracy of the certified value to this level but are given to minimise rounding errors when calculating 2SD

Figure 1. Au by Pb Fire Assay in OREAS 911

SPC.1941.RR1.OREAS 911.2.Fire Assay.Au.Lab.260326.122734.SN

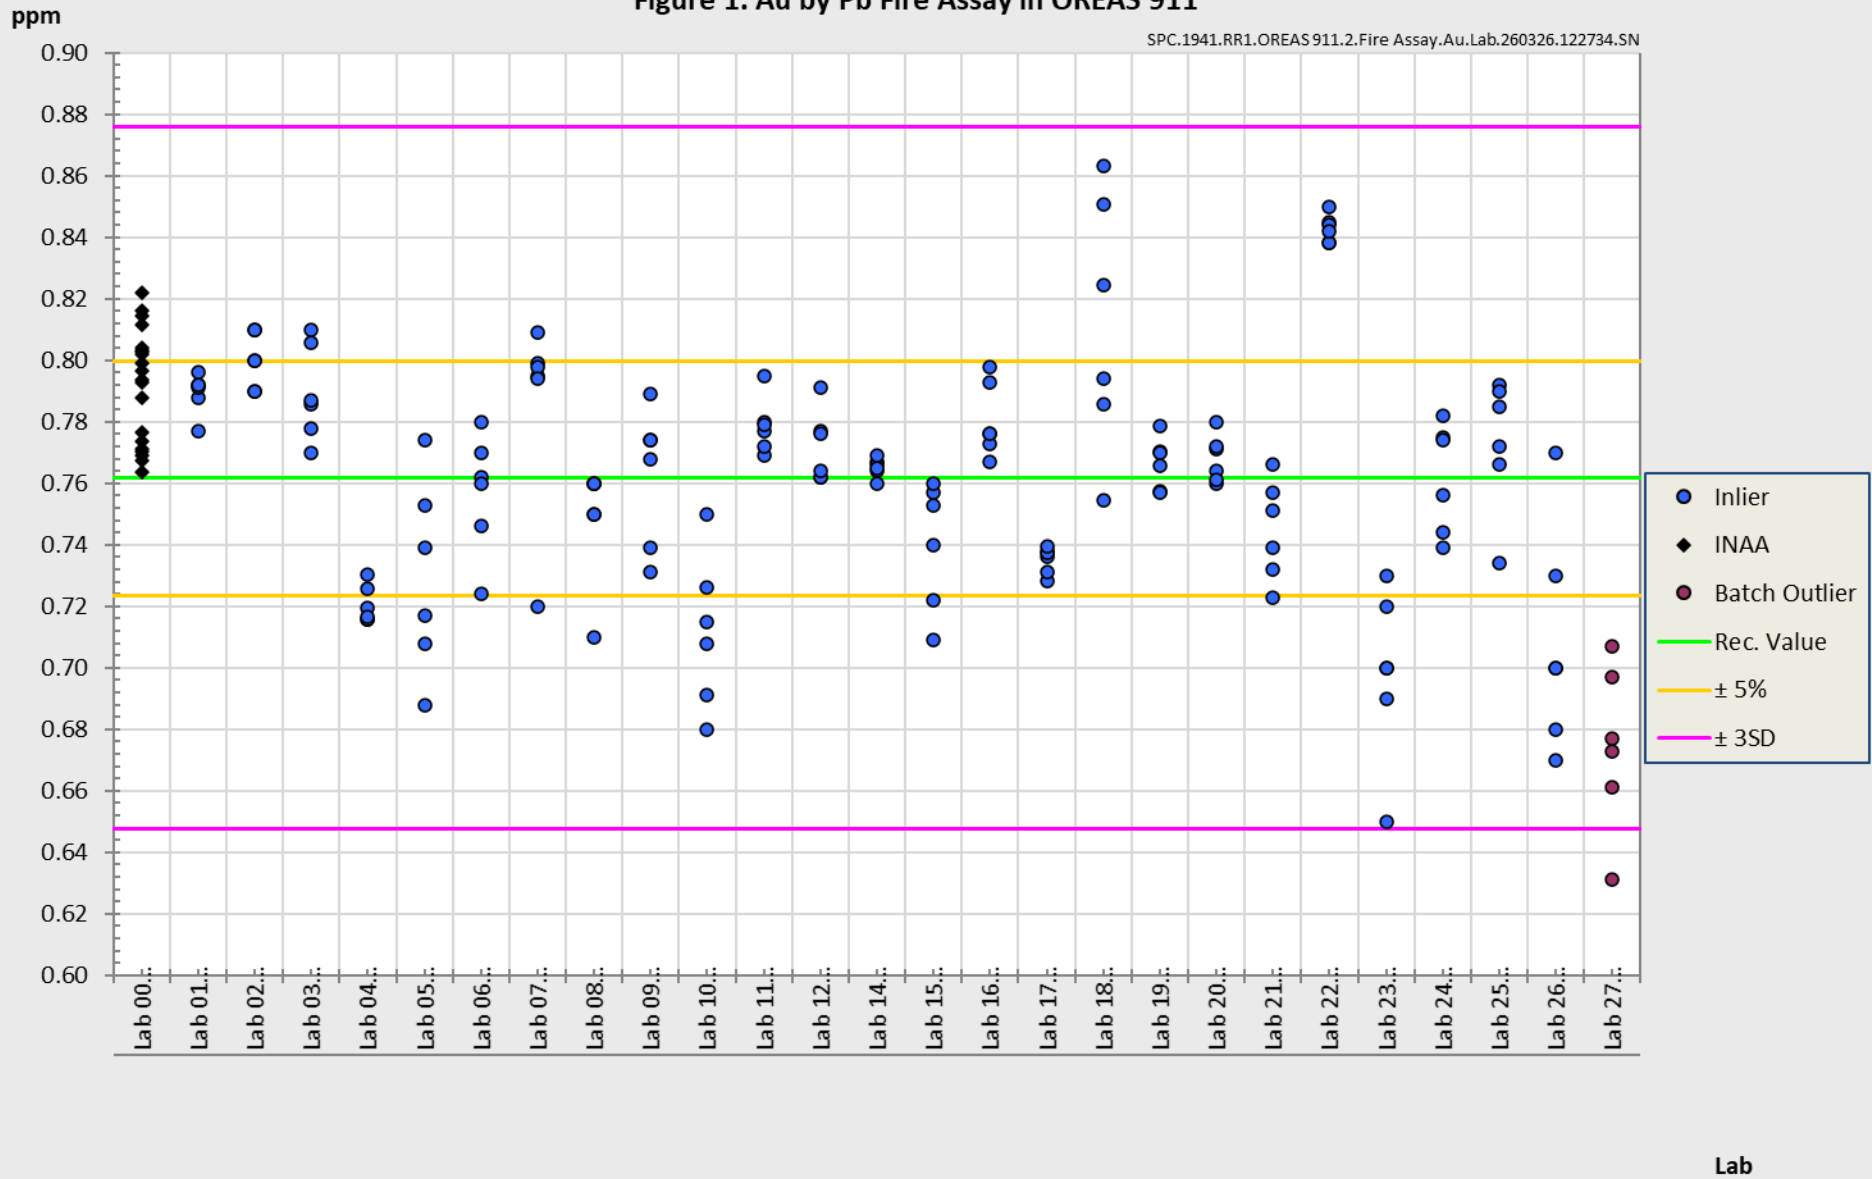


Figure 2. Cu by 4-Acid Digestion in OREAS 911

SPC.1941.RR1.OREAS 911.2.4-Acid.Cu.Lab.260326.123414.SN


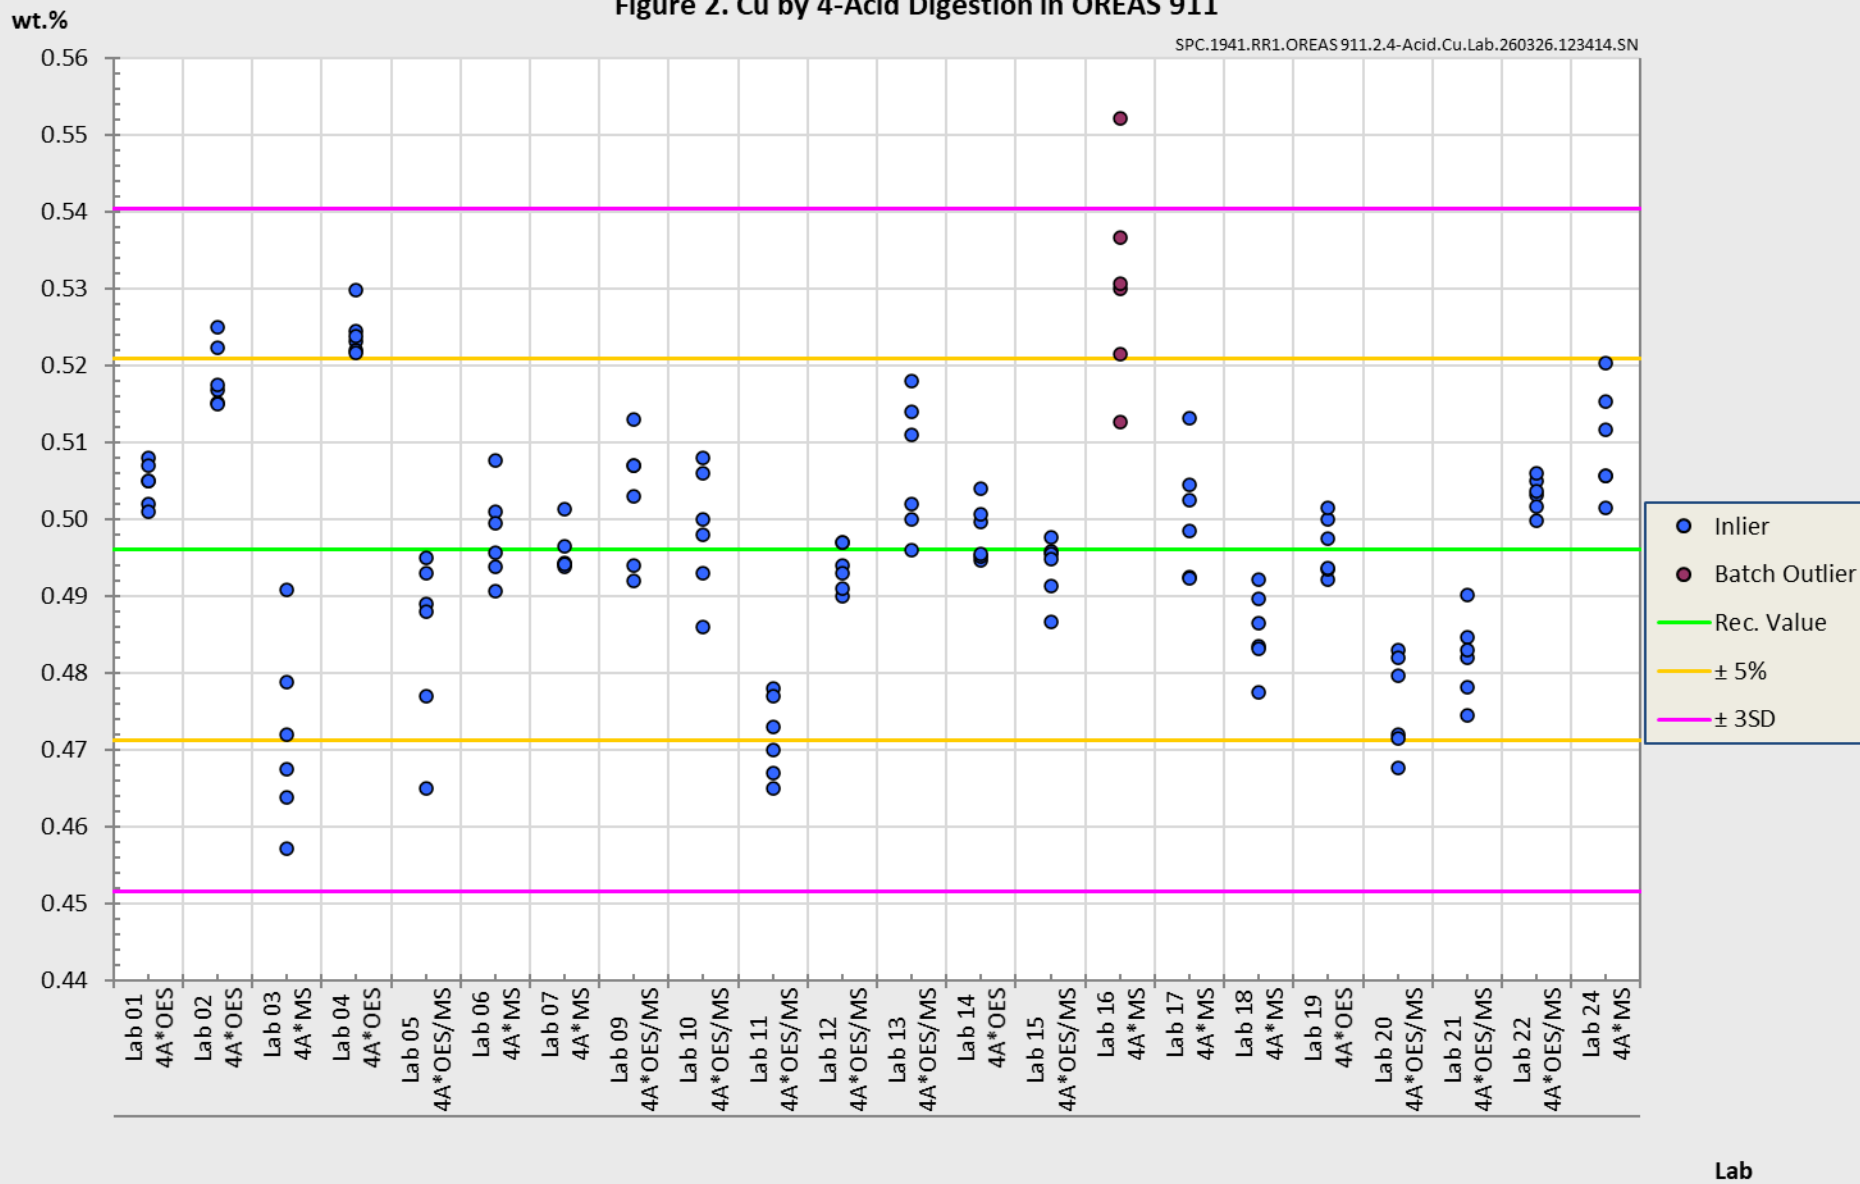


Figure 3. Zn by 4-Acid Digestion in OREAS 911

SPC.1941.RR1.OREAS 911.2.4-Acid.Zn.Lab.260326.123459.SN

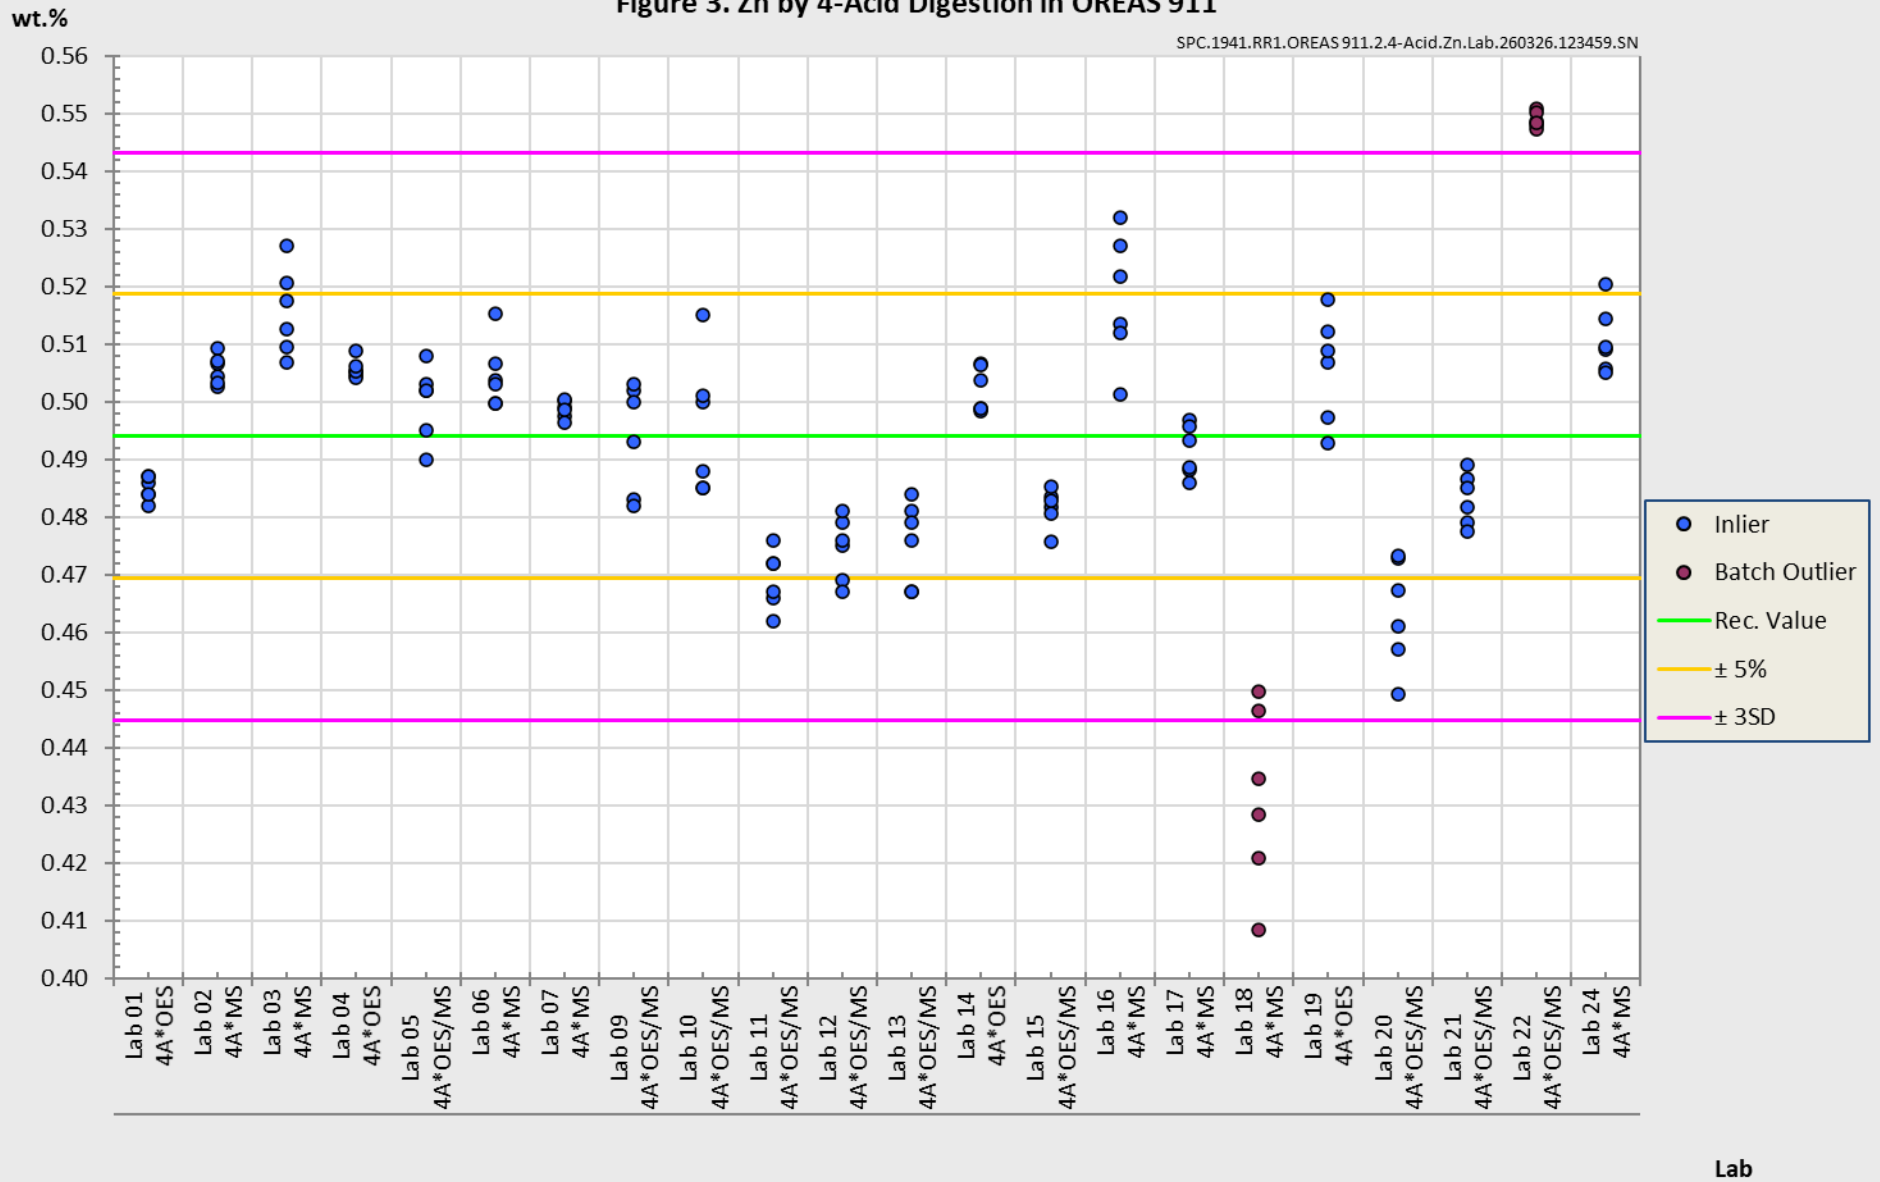

PREPARER AND SUPPLIER

Certified reference material OREAS 911 is prepared, certified and supplied by:

ORE Research & Exploration Pty Ltd
37A Hosie Street
Bayswater North VIC 3153
AUSTRALIA

Tel: +613-9729 0333
Web: www.oreas.com
Email: info@ore.com.au

CERTIFYING OFFICER

Craig Hamlyn (B.Sc. Hons - Geology), Technical Manager - ORE P/L

ACCREDITATION

ORE Pty Ltd is accredited for compliance with ISO 17034:2016 (Accreditation number 20483).



ORE Pty Ltd is ISO 9001:2015 certified by Lloyd's Register Quality Assurance Ltd for its quality management system including development, manufacturing, certification and supply of CRMs.



LEGAL NOTICE

Ore Research & Exploration Pty Ltd has prepared and statistically evaluated the property values of this reference material to the best of its ability. The Purchaser by receipt hereof releases and indemnifies Ore Research & Exploration Pty Ltd from and against all liability and costs arising from the use of this material and information.

© COPYRIGHT Ore Research & Exploration Pty Ltd.
Unauthorised copying, reproduction, storage or dissemination is prohibited.

DOCUMENT HISTORY

Revision No.	Date	Changes applied
0	1 st April 2026	First publication.

REFERENCES

- [1] Govett, G.J.S. (1983). Handbook of Exploration Geochemistry, Volume 2: Statistics and Data Analysis in Geochemical Prospecting (Variations of accuracy and precision).
- [2] Ingamells, C. O. and Switzer, P. (1973). A Proposed Sampling Constant for Use in Geochemical Analysis, *Talanta* 20, 547-568.
- [3] ISO Guide 30:2015. Terms and definitions used in connection with reference materials.
- [4] ISO 33401:2024-01. Reference materials – Contents of certificates, labels and accompanying documentation.
- [5] ISO 33405:2024-05. Reference materials – Approaches for characterization and assessment of homogeneity and stability.
- [6] ISO Guide 98-3:2008. Guide to the expression of uncertainty in measurement (GUM:1995).
- [7] ISO 16269:2014. Statistical interpretation of data – Part 6: Determination of statistical tolerance intervals.
- [8] ISO 17025:2017, General requirements for the competence of testing and calibration laboratories.
- [9] ISO 17034:2016. General requirements for the competence of reference material producers.
- [10] Munsell Rock Color Book (2014). Rock-Color Chart Committee, Geological Society of America (GSA), Minnesota (USA).
- [11] OREAS-BUP-70-09-11: Statistical Analysis - OREAS Evaluation Method.
- [12] OREAS-TN-04-1498: Stability under transport; an experimental study of OREAS CRMs.
- [13] OREAS-TN-05-1674: Long-term storage stability; an experimental study of OREAS CRMs.
- [14] Thompson, A.; Taylor, B.N. (2008); Guide for the Use of the International System of Units (SI); NIST Special Publication 811; U.S. Government Printing Office: Washington, DC; available at: <https://physics.nist.gov/cuu/pdf/sp811.pdf> (accessed Nov 2021).
- [15] Van der Veen A.M.H. et al. (2001). Uncertainty calculations in the certification of reference materials, *Accred Qual Assur* 6: 290-294.